


LB107037
INSTRUMENT ID CV1

7470A

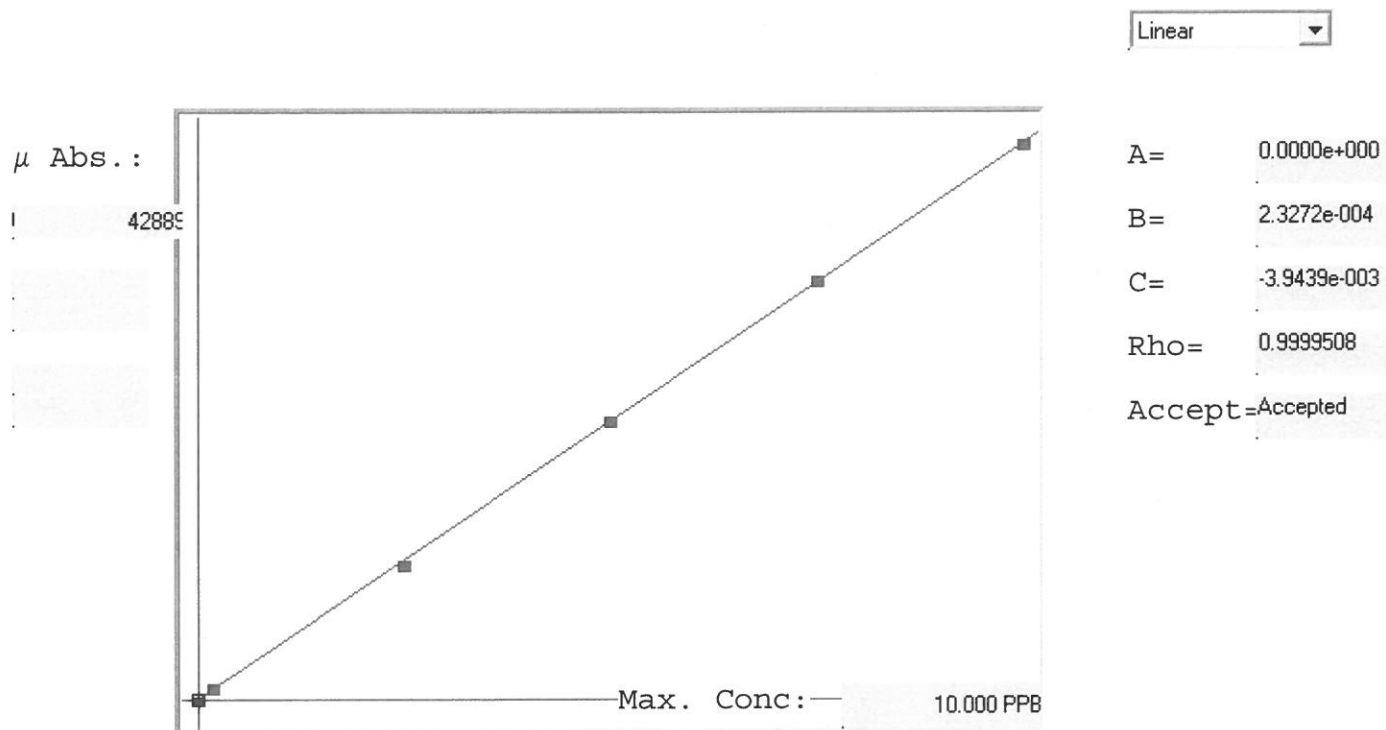

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.010	0.010	60	0.000	60				
0.2	0.200	0.222	0.022	969	0.0 %	969				
2.5	2.500	2.429	-0.071	10455	0.0 %	10455				
5.0	5.000	5.029	0.029	21627	0.0 %	21627				
7.5	7.500	7.533	0.033	32386	0.0 %	32386				
10.0	10.000	9.977	-0.023	42889	0.0 %	42889				

LB107037 INSTRUMENT ID CV1

Method: 7470A		Operator: Admin		Date of Analysis: 06 Jan 2020 11:12:31					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD.0	60	-	0.0000	7470A	PPB	06 Jan 2020 11:14:40	S	Std
0.2 - 1	SD.2	969	-	0.2000	7470A	PPB	06 Jan 2020 11:16:47	S	Std
2.5 - 1	SD.5	10455	-	2.5000	7470A	PPB	06 Jan 2020 11:18:55	S	Std
5.0 - 1	SD.0	21627	-	5.0000	7470A	PPB	06 Jan 2020 11:21:02	S	Std
7.5 - 1	SD.9	32386	-	7.5000	7470A	PPB	06 Jan 2020 11:23:09	S	Std
10.0 - 1	SD.0	42889	-	10.0000	7470A	PPB	06 Jan 2020 11:25:16	S	Std
ICV51 - 1	ICV51	16587	3.8562	-	7470A	PPB	06 Jan 2020 11:27:37	U	SMPL
ICB51 - 1	ICB51	-20	-0.0086	-	7470A	PPB	06 Jan 2020 11:29:42	U	SMPL
CCV16 - 1	CCV16	21933	5.1003	-	7470A	PPB	06 Jan 2020 11:31:48	U	SMPL
CCB16 - 1	CCB16	-1	-0.0042	-	7470A	PPB	06 Jan 2020 11:33:53	U	SMPL
CRA - 1	CRA	946	0.2162	-	7470A	PPB	06 Jan 2020 11:35:59	U	SMPL
HighStd - 1	HighStd	42829	9.9633	-	7470A	PPB	06 Jan 2020 11:38:04	U	SMPL
ChkStd - 1	ChkStd	30894	7.1857	-	7470A	PPB	06 Jan 2020 11:40:10	U	SMPL
PB125901BL - 1	PBW	-43	-0.0140	-	7470A	PPB	06 Jan 2020 11:42:17	U	SMPL
PB125901BS - 1	LCSW	16936	3.9374	-	7470A	PPB	06 Jan 2020 11:44:23	U	SMPL
L1008-02 - 1	CL-02-010220	-22	-0.0091	-	7470A	PPB	06 Jan 2020 11:46:30	U	SMPL
L1008-02DUP - 1	CL-02-010220DUP	-11	-0.0065	-	7470A	PPB	06 Jan 2020 11:48:37	U	SMPL
L1008-02MS - 1	CL-02-010220MS	11526	2.6784	-	7470A	PPB	06 Jan 2020 11:50:45	U	SMPL
L1008-02MSD - 1	CL-02-010220MSD	11735	2.7270	-	7470A	PPB	06 Jan 2020 11:52:53	U	SMPL
L1009-02 - 1	NB-08-010220	-48	-0.0151	-	7470A	PPB	06 Jan 2020 11:54:59	U	SMPL
CCV17 - 1	CCV17	22355	5.1985	-	7470A	PPB	06 Jan 2020 11:57:05	U	SMPL
CCB17 - 1	CCB17	-32	-0.0114	-	7470A	PPB	06 Jan 2020 11:59:11	U	SMPL
L1010-02 - 1	OK-01-010220	-26	-0.0100	-	7470A	PPB	06 Jan 2020 12:01:17	U	SMPL
L1008-02LX5 - 1		-82	-0.0230	-	7470A	PPB	06 Jan 2020 12:03:22	U	SMPL
PB125901TB - 1	PB125869TB	-66	-0.0193	-	7470A	PPB	06 Jan 2020 12:05:28	U	SMPL
L1008-02A - 1		17597	4.0912	-	7470A	PPB	06 Jan 2020 12:07:34	U	SMPL
CCV18 - 1	CCV18	22052	5.1280	-	7470A	PPB	06 Jan 2020 12:09:41	U	SMPL
CCB18 - 1	CCB18	-85	-0.0237	-	7470A	PPB	06 Jan 2020 12:11:48	U	SMPL