


LB 107107
INSTRUMENT ID : CV1

ISM02.4

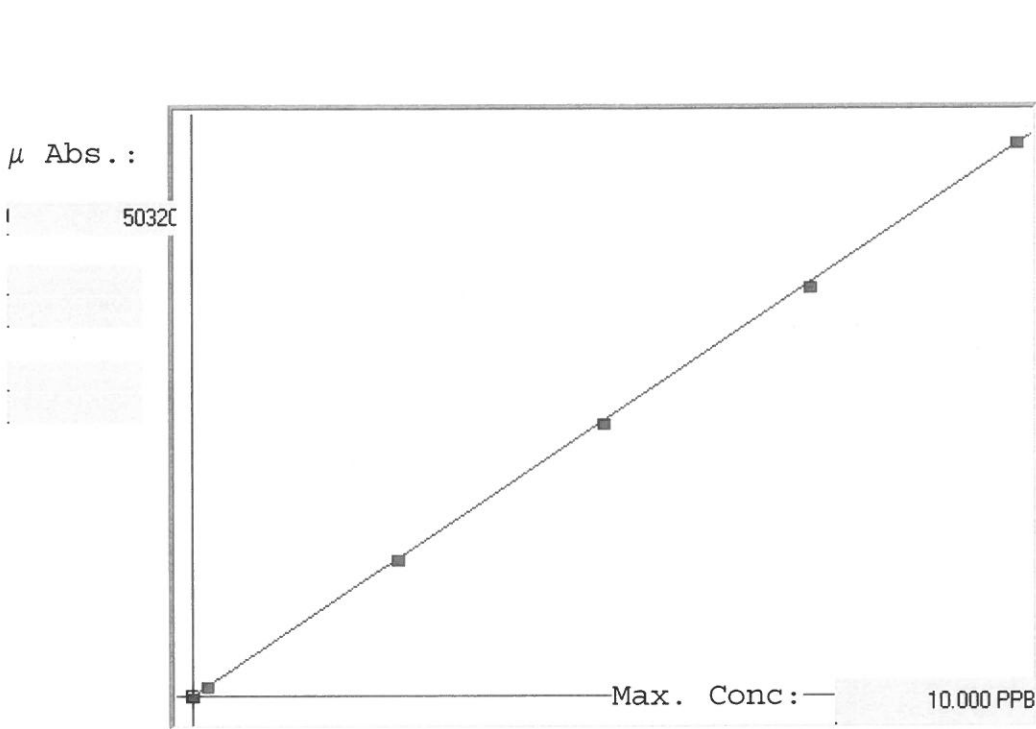

Linear

A= 0.0000e+000

B= 1.9965e-004

C= 1.9627e-002

Rho= 0.9999343

Accept=Accepted

Slope

Intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.016	0.016	-17	0.000	-17					
0.05	0.050										
0.20	0.200	0.219	0.019	1000	0.0 %	1000					10
2.50	2.500	2.502	0.002	12434	0.0 %	12434					0
5.00	5.000	4.961	-0.039	24751	0.0 %	24751					-1
7.50	7.500	7.435	-0.065	37142	0.0 %	37142					-1
10.0	10.000	10.066	0.066	50320	0.0 %	50320					1

01/09/20

(B4)

Sample ID	Extended II μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	
0 S0.0	-17	-	0	ISM02.4	PPB	1/9/2020 16:52	Std	
0.2 S0.2	1000	-	0.2	ISM02.4	PPB	1/9/2020 16:54	Std	
2.5 S2.5	12434	-	2.5	ISM02.4	PPB	1/9/2020 16:57	Std	
5 S5.0	24751	-	5	ISM02.4	PPB	1/9/2020 16:59	Std	
7.5 S7.5	37142	-	7.5	ISM02.4	PPB	1/9/2020 17:01	Std	
10 S10.0	50320	-	10	ISM02.4	PPB	1/9/2020 17:04	Std	
ICV	ICV	20137	4.04	-	ISM02.4	PPB	1/9/2020 17:11	SMPL
ICB	ICB	-44	0.0108	-	ISM02.4	PPB	1/9/2020 17:13	SMPL
CCV035	CCV035	24256	4.8624	-	ISM02.4	PPB	1/9/2020 17:15	SMPL
CCB035	CCB035	-74	0.0049	-	ISM02.4	PPB	1/9/2020 17:17	SMPL
PB125968E	PBS596	14	0.0224	-	ISM02.4	PPB	1/9/2020 17:20	SMPL
K6451-01	MA5481	3963	0.8108	-	ISM02.4	PPB	1/9/2020 17:22	SMPL
K6451-02	MA5482	127	0.045	-	ISM02.4	PPB	1/9/2020 17:24	SMPL
CCV036	CCV036	24297	4.8706	-	ISM02.4	PPB	1/9/2020 17:26	SMPL
CCB036	CCB036	-10	0.0176	-	ISM02.4	PPB	1/9/2020 17:29	SMPL