


LB 107190 INSTRUMENT ID: CV1

245.1

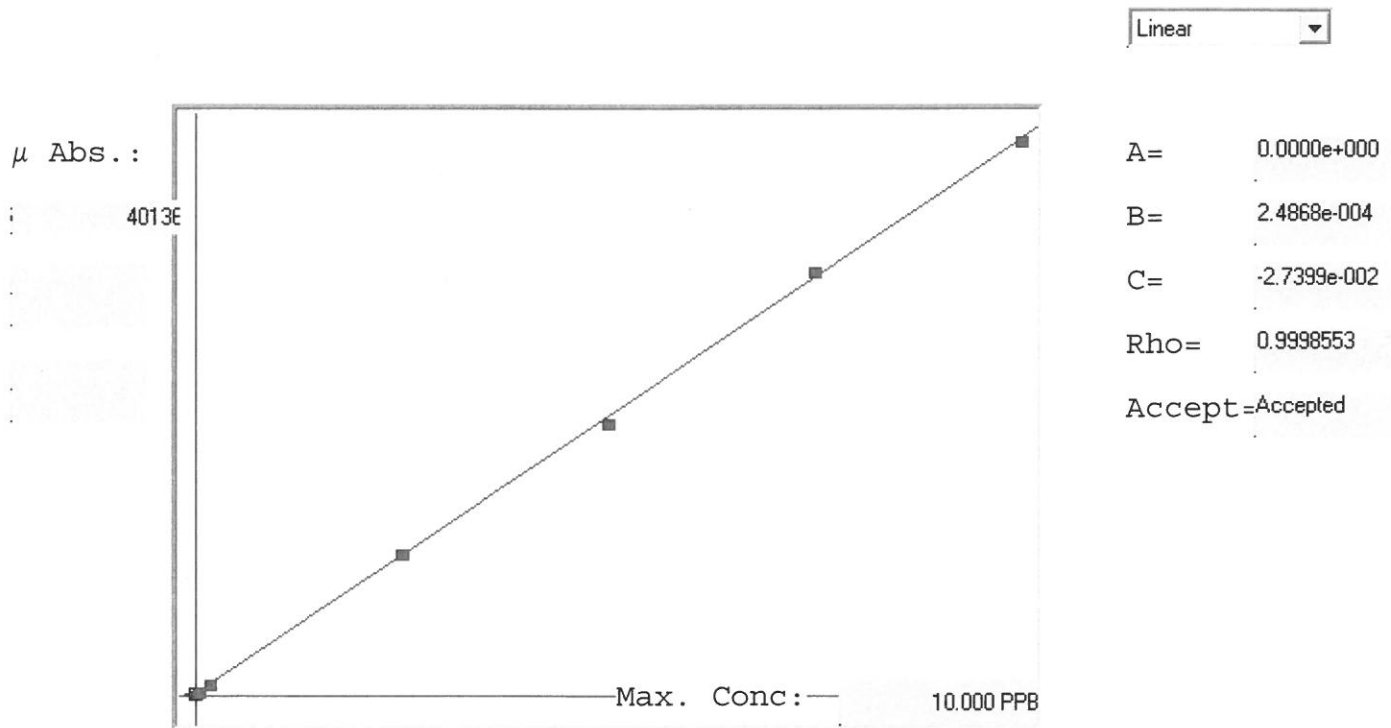

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.015	0.015	169	0.000	169				
0.05	0.050	0.043	-0.007	283	0.0 %	283				
0.2	0.200	0.180	-0.020	836	0.0 %	836				
2.5	2.500	2.550	0.050	10366	0.0 %	10366				
5.0	5.000	4.898	-0.102	19806	0.0 %	19806				
7.5	7.500	7.610	0.110	30713	0.0 %	30713				
10.0	10.000	9.953	-0.047	40136	0.0 %	40136				

LB107190 INSTRUMENT ID :CV1

Method: 245.1

Operator: Admin

Date of Analysis: 15 Jan 2020 18:14:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD-0	169	-	0.0000	245.1	PPB	15 Jan 2020 18:19:24	S	Std
0.05 - 1	SD-05	283	-	0.0500	245.1	PPB	15 Jan 2020 18:21:41	S	Std
0.2 - 1	SD-2	836	-	0.2000	245.1	PPB	15 Jan 2020 18:23:59	S	Std
2.5 - 1	SD-5	10366	-	2.5000	245.1	PPB	15 Jan 2020 18:26:15	S	Std
5.0 - 1	SD-7	19806	-	5.0000	245.1	PPB	15 Jan 2020 18:28:32	S	Std
7.5 - 1	SD-7.5	30713	-	7.5000	245.1	PPB	15 Jan 2020 18:30:48	S	Std
10.0 - 1	SD-10	40136	-	10.0000	245.1	PPB	15 Jan 2020 18:44:25	S	Std
ICV70 - 1	ICV70	15491	3.8248	-245.1		PPB	15 Jan 2020 18:49:18	U	SMPL
ICB70 - 1	ICB70	120	0.0024	-245.1		PPB	15 Jan 2020 18:51:33	U	SMPL
CCV59 - 1	CCV59	20290	5.0182	-245.1		PPB	15 Jan 2020 18:53:47	U	SMPL
CCB59 - 1	CCB59	98	-0.0030	-245.1		PPB	15 Jan 2020 18:56:02	U	SMPL
CRA - 1	CRA	292	0.0452	-245.1		PPB	15 Jan 2020 18:58:17	U	SMPL
HighStd - 1	HighStd	41109	10.1954	-245.1		PPB	15 Jan 2020 19:00:32	U	SMPL
ChkStd - 1	ChkStd	28805	7.1357	-245.1		PPB	15 Jan 2020 19:06:21	U	SMPL
PB126119BL - 1	PBW	118	0.0019	-245.1		PPB	15 Jan 2020 19:08:36	U	SMPL
PB126119BS - 1	LCSW	16620	4.1056	-245.1		PPB	15 Jan 2020 19:10:51	U	SMPL
L1018-02 - 1	COMP	163	0.0131	-245.1		PPB	15 Jan 2020 19:13:08	U	SMPL
L1102-02 - 1	EFF-WW	184	0.0184	-245.1		PPB	15 Jan 2020 19:15:24	U	SMPL
L1102-02DUP - 1	EFF-WWDUP	191	0.0201	-245.1		PPB	15 Jan 2020 19:17:41	U	SMPL
L1102-02MS - 1	EFF-WWMS	16824	4.1563	-245.1		PPB	15 Jan 2020 19:19:58	U	SMPL
L1102-02MSD - 1	EFF-WWMSD	16926	4.1817	-245.1		PPB	15 Jan 2020 19:22:13	U	SMPL
CCV60 - 1	CCV60	20604	5.0963	-245.1		PPB	15 Jan 2020 19:28:15	U	SMPL
CCB60 - 1	CCB60	124	0.0034	-245.1		PPB	15 Jan 2020 19:30:30	U	SMPL
L1123-13 - 1	TWP-01	537	0.1061	-245.1		PPB	15 Jan 2020 19:32:46	U	SMPL
L1126-07 - 1	FB-01142020	180	0.0174	-245.1		PPB	15 Jan 2020 19:35:01	U	SMPL
L1102-02LX5 - 1		31	-0.0197	-245.1		PPB	15 Jan 2020 19:37:17	U	SMPL
CCV61 - 1	CCV61	20650	5.1078	-245.1		PPB	15 Jan 2020 19:39:33	U	SMPL
CCB61 - 1	CCB61	-12	-0.0304	-245.1		PPB	15 Jan 2020 19:41:49	U	SMPL