


LB 107204

7470A

INSTRUMENT ID: CVI

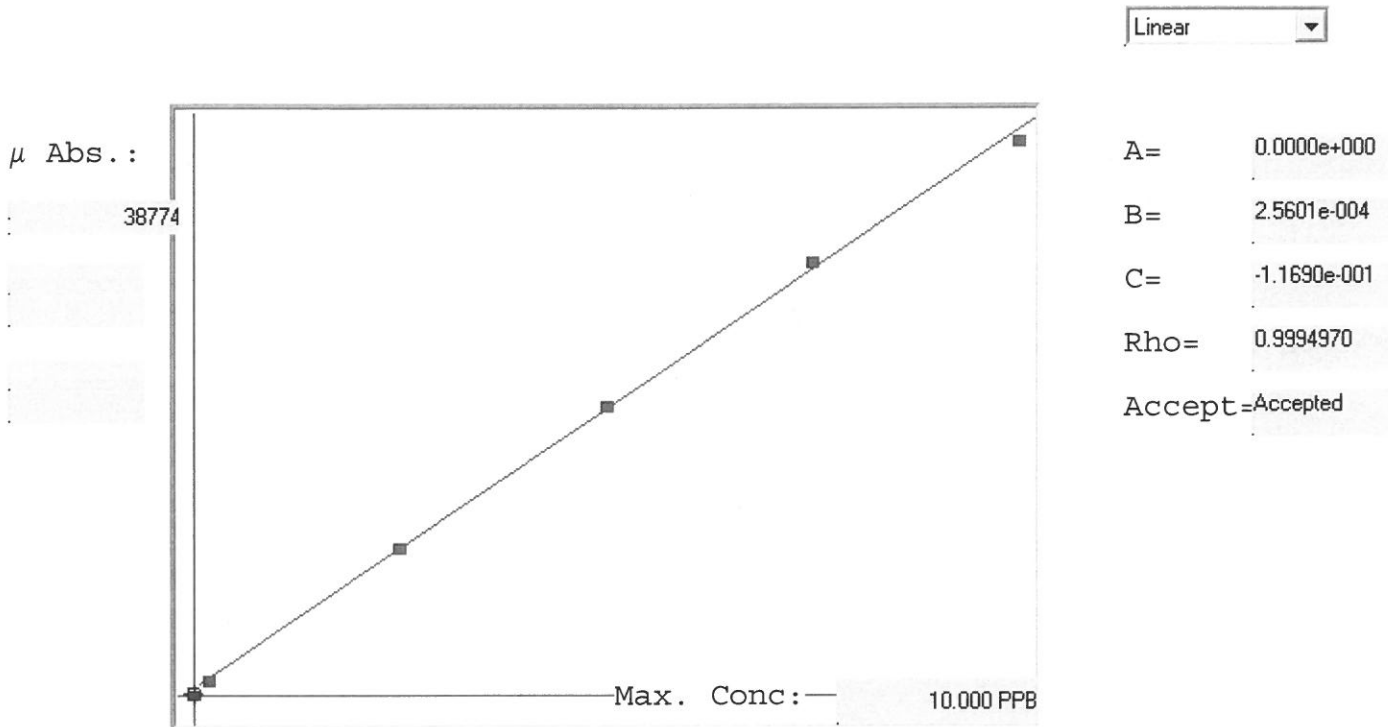

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.066	-0.066	199	0.000	199				
0.2	0.200	0.158	-0.042	1075	0.0 %	1075				
2.5	2.500	2.543	0.043	10391	0.0 %	10391				
5.0	5.000	5.075	0.075	20282	0.0 %	20282				
7.5	7.500	7.680	0.180	30454	0.0 %	30454				
10.0	10.000	9.809	-0.191	38774	0.0 %	38774				

LB107204 INSTRUMENT ID:CV1

Method: 7470A		Operator: Admin		Date of Analysis: 16 Jan 2020 16:33:27				
Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	SD-0	199	-	0.0000	7470A	PPB	16 Jan 2020 16:35:10	S Std
0.2 - 1	SD-2	1075	-	0.2000	7470A	PPB	16 Jan 2020 16:37:17	S Std
2.5 - 1	SD-5	10391	-	2.5000	7470A	PPB	16 Jan 2020 16:39:24	S Std
5.0 - 1	SD-10	20282	-	5.0000	7470A	PPB	16 Jan 2020 16:41:32	S Std
7.5 - 1	SD-15	30454	-	7.5000	7470A	PPB	16 Jan 2020 16:43:39	S Std
10.0 - 1	SD-20	38774	-	10.0000	7470A	PPB	16 Jan 2020 16:45:45	S Std
ICV71 - 1	ICV71	16432	4.0898	-	7470A	PPB	16 Jan 2020 16:49:02	U SMPL
ICB71 - 1	ICB71	154	-0.0775	-	7470A	PPB	16 Jan 2020 16:51:07	U SMPL
CCV62 - 1	CCV62	21017	5.2636	-	7470A	PPB	16 Jan 2020 16:53:13	U SMPL
CCB62 - 1	CCB62	146	-0.0795	-	7470A	PPB	16 Jan 2020 16:55:18	U SMPL
CRA - 1	CRA	1133	0.1732	-	7470A	PPB	16 Jan 2020 17:06:51	U SMPL
HighStd - 1	HighStd	39778	10.0665	-	7470A	PPB	16 Jan 2020 17:08:56	U SMPL
ChkStd - 1	ChkStd	27039	6.8052	-	7470A	PPB	16 Jan 2020 17:11:02	U SMPL
PB126142BL - 1	PB126142BL PBW	150	-0.0785	-	7470A	PPB	16 Jan 2020 17:13:09	U SMPL
PB126142BS - 1	PB126142BS LCSW	17653	4.4024	-	7470A	PPB	16 Jan 2020 17:20:04	U SMPL
L1006-04 - 1	HD-01-011520	210	-0.0631	-	7470A	PPB	16 Jan 2020 17:22:10	U SMPL
L1016-09 - 1	SU-03-011520	207	-0.0639	-	7470A	PPB	16 Jan 2020 17:24:17	U SMPL
L1017-06 - 1	TR-05-011520	203	-0.0649	-	7470A	PPB	16 Jan 2020 17:26:24	U SMPL
L1126-06 - 1	WASTE-CHARACTERIZATION	166	-0.0744	-	7470A	PPB	16 Jan 2020 17:28:32	U SMPL
L1126-06MS - 1	WASTE-CHARACTERIZATIONMS	14949	3.7101	-	7470A	PPB	16 Jan 2020 17:30:38	U SMPL
CCV63 - 1	CCV63	20465	5.1223	-	7470A	PPB	16 Jan 2020 17:32:44	U SMPL
CCB63 - 1	CCB63	150	-0.0785	-	7470A	PPB	16 Jan 2020 17:34:50	U SMPL
L1126-06MSD - 1	WASTE-CHARACTERIZATIONMSD	16010	3.9818	-	7470A	PPB	16 Jan 2020 17:36:56	U SMPL
L1138-01 - 1	SB-1-(5-7)	199	-0.0660	-	7470A	PPB	16 Jan 2020 17:39:02	U SMPL
L1138-02 - 1	SB-3-(3-4)	218	-0.0611	-	7470A	PPB	16 Jan 2020 17:41:08	U SMPL
L1138-03 - 1	SB-5-(0-2)	185	-0.0695	-	7470A	PPB	16 Jan 2020 17:43:14	U SMPL
PB126120BL - 1	PB126120BL PBW	144	-0.0800	-	7470A	PPB	16 Jan 2020 17:45:21	U SMPL
PB126120BS - 1	PB126120BS LCSW	16744	4.1697	-	7470A	PPB	16 Jan 2020 17:47:28	U SMPL
L1005-05 - 1	HR-05-011420	171	-0.0731	-	7470A	PPB	16 Jan 2020 17:49:35	U SMPL
L1005-05DUP - 1	HR-05-011420DUP	184	-0.0698	-	7470A	PPB	16 Jan 2020 17:51:43	U SMPL
L1005-05MS - 1	HR-05-011420MS	18999	4.7470	-	7470A	PPB	16 Jan 2020 17:53:50	U SMPL
L1005-05MSD - 1	HR-05-011420MSD	18648	4.6571	-	7470A	PPB	16 Jan 2020 17:55:57	U SMPL
CCV64 - 1	CCV64	20371	5.0982	-	7470A	PPB	16 Jan 2020 17:58:03	U SMPL
CCB64 - 1	CCB64	138	-0.0816	-	7470A	PPB	16 Jan 2020 18:00:09	U SMPL
L1123-09 - 1	SB-01-COMP	199	-0.0660	-	7470A	PPB	16 Jan 2020 18:02:15	U SMPL
L1123-10 - 1	SB-02-COMP	188	-0.0688	-	7470A	PPB	16 Jan 2020 18:04:22	U SMPL
L1123-11 - 1	SB-03-COMP	178	-0.0713	-	7470A	PPB	16 Jan 2020 18:06:28	U SMPL
L1123-12 - 1	SB-04-COMP	189	-0.0685	-	7470A	PPB	16 Jan 2020 18:08:34	U SMPL
PB126093BL - 1	PB126093BL PBW	147	-0.0793	-	7470A	PPB	16 Jan 2020 18:10:40	U SMPL
PB126093BS - 1	PB126093BS LCSW	17180	4.2813	-	7470A	PPB	16 Jan 2020 18:23:42	U SMPL
L1004-03 - 1	BU-RO-258	173	-0.0726	-	7470A	PPB	16 Jan 2020 18:25:49	U SMPL
L1004-06 - 1	BU-RO-234	185	-0.0695	-	7470A	PPB	16 Jan 2020 18:27:56	U SMPL
L1004-06DUP - 1	BU-RO-234DUP	198	-0.0662	-	7470A	PPB	16 Jan 2020 18:30:03	U SMPL
L1004-06MS - 1	BU-RO-234MS	13887	3.4383	-	7470A	PPB	16 Jan 2020 18:32:09	U SMPL
CCV65 - 1	CCV65	20088	5.0257	-	7470A	PPB	16 Jan 2020 18:34:15	U SMPL
CCB65 - 1	CCB65	140	-0.0811	-	7470A	PPB	16 Jan 2020 18:36:21	U SMPL
L1004-06MSD - 1	BU-RO-234MSD	12866	3.1769	-	7470A	PPB	16 Jan 2020 18:38:27	U SMPL
L1004-09 - 1	BU-RO-229	227	-0.0588	-	7470A	PPB	16 Jan 2020 18:40:33	U SMPL
L1111-02 - 1	OUTSIDE-BRICK	155	-0.0772	-	7470A	PPB	16 Jan 2020 18:42:39	U SMPL
L1111-05 - 1	OUTSIDE-FOUNDATIONS	169	-0.0736	-	7470A	PPB	16 Jan 2020 18:44:46	U SMPL
L1111-08 - 1	CONCRETE-FLOOR	173	-0.0726	-	7470A	PPB	16 Jan 2020 18:46:52	U SMPL
PB126142TB - 1	PB126142TB	166	-0.0744	-	7470A	PPB	16 Jan 2020 18:48:59	U SMPL
PB126120TB - 1	PB126096TB	194	-0.0672	-	7470A	PPB	16 Jan 2020 18:51:07	U SMPL
PB126093TB - 1	PB126093TB	116	-0.0872	-	7470A	PPB	16 Jan 2020 18:53:14	U SMPL
L1126-06DUP - 1		139	-0.0813	-	7470A	PPB	16 Jan 2020 18:55:21	U SMPL
L1126-06LX5 - 1		31	-0.1090	-	7470A	PPB	16 Jan 2020 18:57:27	U SMPL
CCV66 - 1	CCV66	20224	5.0606	-	7470A	PPB	16 Jan 2020 18:59:33	U SMPL
CCB66 - 1	CCB66	138	-0.0816	-	7470A	PPB	16 Jan 2020 19:01:40	U SMPL
L1005-05LX5 - 1		26	-0.1102	-	7470A	PPB	16 Jan 2020 19:03:46	U SMPL
L1004-06LX5 - 1		35	-0.1079	-	7470A	PPB	16 Jan 2020 19:05:52	U SMPL
CCV67 - 1	CCV67	19979	4.9978	-	7470A	PPB	16 Jan 2020 19:07:58	U SMPL
CCB67 - 1	CCB67	129	-0.0839	-	7470A	PPB	16 Jan 2020 19:10:04	U SMPL

BAP

d/16/20