


LB107230

7471B

INSTRUMENT ID: CV1

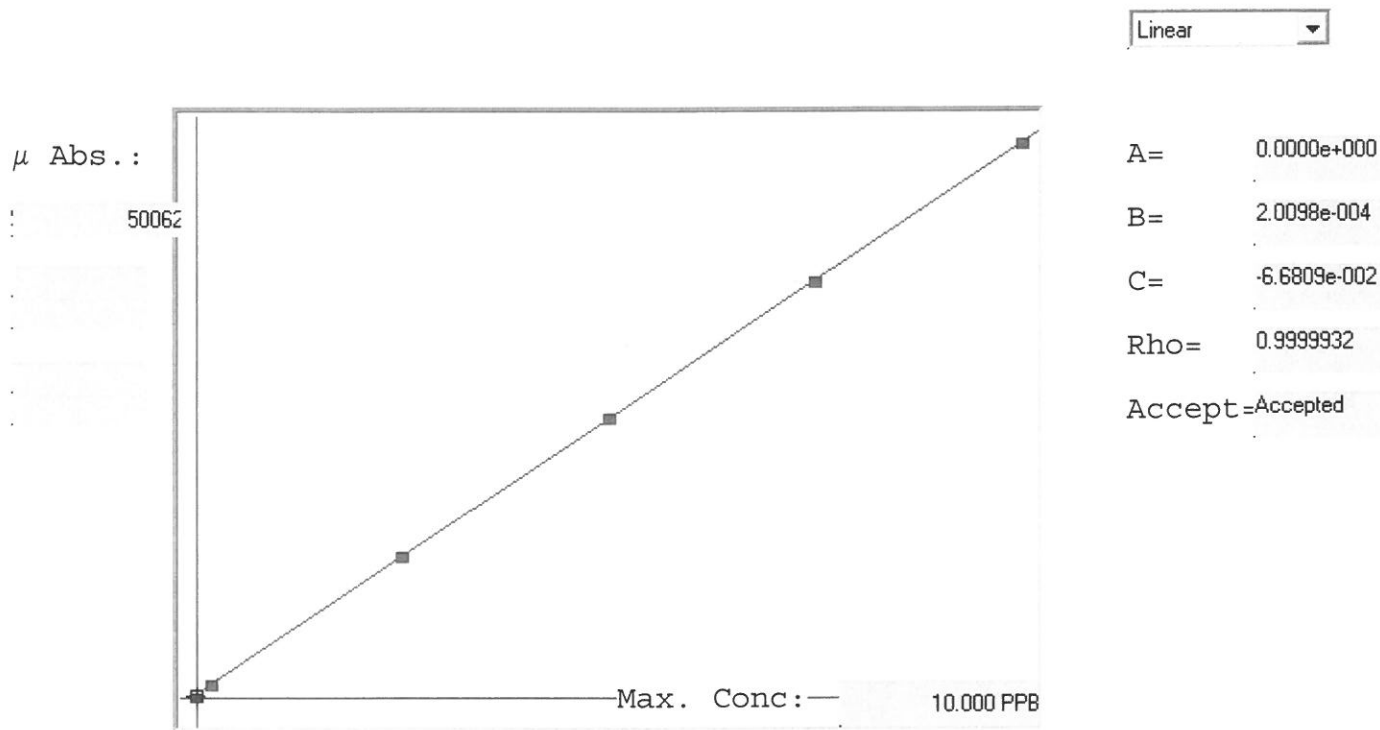

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.013	-0.013	269	0.000	269				
0.2	0.200	0.192	-0.008	1290	0.0 %	1290				
2.5	2.500	2.517	0.017	12858	0.0 %	12858				
5.0	5.000	5.021	0.021	25313	0.0 %	25313				
7.5	7.500	7.488	-0.012	37590	0.0 %	37590				
10.0	10.000	9.995	-0.005	50062	0.0 %	50062				

LB107230 INSTRUMENT ID :CV1

Method: 7471B		Operator: Admin		Date of Analysis: 17 Jan 2020 14:34:28				
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	SD.D	269	-	0.00007471B	PPB		17 Jan 2020 14:48:45	S Std
0.2 - 1	SD.2	1290	-	0.20007471B	PPB		17 Jan 2020 14:51:02	S Std
2.5 - 1	SD.5	12858	-	2.50007471B	PPB		17 Jan 2020 14:53:18	S Std
5.0 - 1	SD.10	25313	-	5.00007471B	PPB		17 Jan 2020 14:55:35	S Std
7.5 - 1	SD.5	37590	-	7.50007471B	PPB		17 Jan 2020 14:57:51	S Std
10.0 - 1	SD.10	50062	-	10.00007471B	PPB		17 Jan 2020 15:21:51	S Std
ICV72 - 1	ICV72	20756	4.1047	-7471B	PPB		17 Jan 2020 15:24:33	U SMPL
ICB72 - 1	ICB72	157	-0.0353	-7471B	PPB		17 Jan 2020 15:26:48	U SMPL
CCV68 - 1	CCV68	25108	4.9793	-7471B	PPB		17 Jan 2020 15:29:03	U SMPL
CCB68 - 1	CCB68	134	-0.0399	-7471B	PPB		17 Jan 2020 15:31:18	U SMPL
CRA - 1	CRA	1210	0.1764	-7471B	PPB		17 Jan 2020 15:33:34	U SMPL
HighStd - 1	HighStd	50487	10.0799	-7471B	PPB		17 Jan 2020 15:35:48	U SMPL
ChkStd - 1	ChkStd	33636	6.6933	-7471B	PPB		17 Jan 2020 15:38:04	U SMPL
PB126123BL - 1	PBS	114	-0.0439	-7471B	PPB		17 Jan 2020 15:40:22	U SMPL
PB126123BS - 1	LCSS	21037	4.1611	-7471B	PPB		17 Jan 2020 15:42:40	U SMPL
L1006-01 - 1	HD-01-011520	387	0.0110	-7471B	PPB		17 Jan 2020 15:44:55	U SMPL
L1016-05 - 1	SU-03-011520	2738	0.4835	-7471B	PPB		17 Jan 2020 15:47:12	U SMPL
L1017-04 - 1	TR-05-011520	3486	0.6338	-7471B	PPB		17 Jan 2020 15:49:29	U SMPL
L1142-01 - 1	SS-1	5787	1.0962	-7471B	PPB		17 Jan 2020 15:51:46	U SMPL
L1148-01 - 1	SB-10-(7-9)	3730	0.6828	-7471B	PPB		17 Jan 2020 15:54:02	U SMPL
CCV69 - 1	CCV69	24755	4.9084	-7471B	PPB		17 Jan 2020 15:56:16	U SMPL
CCB69 - 1	CCB69	115	-0.0437	-7471B	PPB		17 Jan 2020 15:58:32	U SMPL
L1148-02 - 1	SB-11-(5-7)	7458	1.4321	-7471B	PPB		17 Jan 2020 16:00:49	U SMPL
L1148-03 - 1	SB-12-(4-6)	3954	0.7279	-7471B	PPB		17 Jan 2020 16:03:04	U SMPL
L1148-04 - 1	SB-13-(4-6)	5608	1.0603	-7471B	PPB		17 Jan 2020 16:05:20	U SMPL
L1148-05 - 1	SB-26-(4-6)	705	0.0749	-7471B	PPB		17 Jan 2020 16:07:35	U SMPL
L1148-05DUP - 1	SB-26-(4-6)DUP	754	0.0847	-7471B	PPB		17 Jan 2020 16:09:51	U SMPL
L1148-05MS - 1	SB-26-(4-6)MS	19096	3.7710	-7471B	PPB		17 Jan 2020 16:18:42	U SMPL
L1148-05MSD - 1	SB-26-(4-6)MSD	20466	4.0464	-7471B	PPB		17 Jan 2020 16:28:00	U SMPL
L1148-06 - 1	SB-27-(4-6)	36500	7.2689	-7471B	PPB		17 Jan 2020 16:30:17	U SMPL
L1148-07 - 1	SB-28-(4-6)	1334	0.2013	-7471B	PPB		17 Jan 2020 16:32:34	U SMPL
L1148-08 - 1	SB-29-(4-6)	570	0.0477	-7471B	PPB		17 Jan 2020 16:34:49	U SMPL
CCV70 - 1	CCV70	25013	4.9602	-7471B	PPB		17 Jan 2020 16:37:05	U SMPL
CCB70 - 1	CCB70	100	-0.0467	-7471B	PPB		17 Jan 2020 16:39:20	U SMPL
L1148-09 - 1	SB-30-(3-5)	17509	3.4521	-7471B	PPB		17 Jan 2020 16:41:37	U SMPL
L1148-10 - 1	SB-31-(2-4)	7460	1.4325	-7471B	PPB		17 Jan 2020 16:43:53	U SMPL
L1148-11 - 1	SB-32-(3-5)	8301	1.6015	-7471B	PPB		17 Jan 2020 16:46:08	U SMPL
L1148-12 - 1	SB-33-(5-7)	13231	2.5923	-7471B	PPB		17 Jan 2020 16:48:23	U SMPL
L1148-13 - 1	SB-34-(4-6)	46539	9.2865	-7471B	PPB		17 Jan 2020 16:50:39	U SMPL
L1148-14 - 1	SB-35-(5-7)	7304	1.4011	-7471B	PPB		17 Jan 2020 16:52:55	U SMPL
L1148-15 - 1	SB-36-(7-9)	23571	4.6704	-7471B	PPB		17 Jan 2020 16:55:13	U SMPL
L1148-16 - 1	SB-43-(2-4)	26213	5.2014	-7471B	PPB		17 Jan 2020 16:57:29	U SMPL
L1148-17 - 1	SB-44-(2-4)	57885	11.5667	-7471B	PPB		17 Jan 2020 16:59:46	U SMPL
L1148-18 - 1	SB-49-(0.5-2)	42428	8.4602	-7471B	PPB		17 Jan 2020 17:02:02	U SMPL
CCV71 - 1	CCV71	24607	4.8786	-7471B	PPB		17 Jan 2020 17:04:17	U SMPL
CCB71 - 1	CCB71	56	-0.0556	-7471B	PPB		17 Jan 2020 17:06:34	U SMPL
PB126162BL - 1	PBS	171	-0.0324	-7471B	PPB		17 Jan 2020 17:08:51	U SMPL
PB126162BS - 1	LCSS	21046	4.1630	-7471B	PPB		17 Jan 2020 17:11:06	U SMPL
L1008-08 - 1	CL-01-011620	2008	0.3368	-7471B	PPB		17 Jan 2020 17:13:21	U SMPL
L1008-08DUP - 1	CL-01-011620DUP	2107	0.3566	-7471B	PPB		17 Jan 2020 17:15:37	U SMPL
L1008-08MS - 1	CL-01-011620MS	21016	4.1569	-7471B	PPB		17 Jan 2020 17:23:47	U SMPL
L1008-08MSD - 1	CL-01-011620MSD	21706	4.2956	-7471B	PPB		17 Jan 2020 17:26:03	U SMPL
L1010-06 - 1	OK-02-011620	1822	0.2994	-7471B	PPB		17 Jan 2020 17:28:20	U SMPL
L1012-01 - 1	EO-02-011620	12300	2.4052	-7471B	PPB		17 Jan 2020 17:30:37	U SMPL
L1154-01 - 1	B4-0-15	1953	0.3257	-7471B	PPB		17 Jan 2020 17:32:54	U SMPL
L1154-03 - 1	B4-15-20	852	0.1044	-7471B	PPB		17 Jan 2020 17:35:10	U SMPL
CCV72 - 1	CCV72	24606	4.8784	-7471B	PPB		17 Jan 2020 17:37:25	U SMPL
CCB72 - 1	CCB72	132	-0.0403	-7471B	PPB		17 Jan 2020 17:39:41	U SMPL
L1154-05 - 1	B3-0-15	2049	0.3450	-7471B	PPB		17 Jan 2020 17:41:57	U SMPL
L1154-07 - 1	B3-15-20	22	-0.0624	-7471B	PPB		17 Jan 2020 17:44:12	U SMPL
L1155-01 - 1	RBR-200028	967	0.1275	-7471B	PPB		17 Jan 2020 17:46:28	U SMPL
L1155-04 - 1	RBR-200052	1659	0.2666	-7471B	PPB		17 Jan 2020 17:48:43	U SMPL
L1171-01 - 1	BW-1A-20.0	418	0.0172	-7471B	PPB		17 Jan 2020 17:50:58	U SMPL
L1171-02 - 1	BW-1A-45.0	606	0.0550	-7471B	PPB		17 Jan 2020 17:53:15	U SMPL
L1172-01 - 1	TSP-01	2266	0.3886	-7471B	PPB		17 Jan 2020 17:55:31	U SMPL
L1148-05LX5 - 1		109	-0.0449	-7471B	PPB		17 Jan 2020 17:57:48	U SMPL
L1008-08LX5 - 1		-12	-0.0692	-7471B	PPB		17 Jan 2020 18:00:05	U SMPL
L1148-17DLX10 - 1		5266	0.9915	-7471B	PPB		17 Jan 2020 18:02:20	U SMPL
CCV73 - 1	CCV73	25130	4.9837	-7471B	PPB		17 Jan 2020 18:04:35	U SMPL
CCB73 - 1	CCB73	118	-0.0431	-7471B	PPB		17 Jan 2020 18:06:51	U SMPL