


LB 107410
INSTRUMENT ID: CVI

7470A

Linear

μ Abs.:

4142E

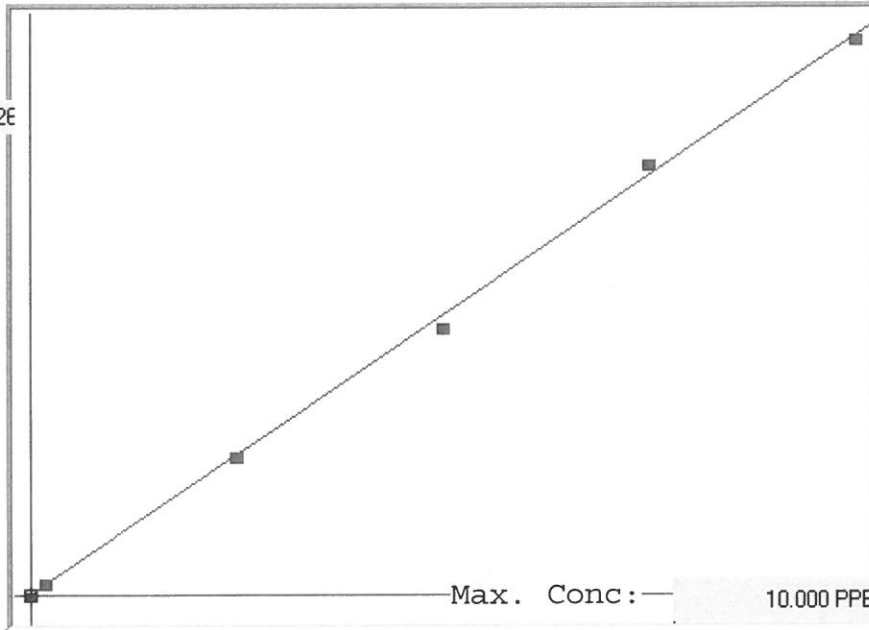

A= 0.0000e+000

B= 2.3982e-004

C= -1.1825e-003

Rho= 0.9994214

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.029	0.029	125	0.000	125				
0.2	0.200	0.239	0.039	1002	0.0 %	1002				
2.5	2.500	2.487	-0.013	10376	0.0 %	10376				
5.0	5.000	4.796	-0.204	20005	0.0 %	20005				
7.5	7.500	7.715	0.215	32174	0.0 %	32174				
10.0	10.000	9.934	-0.066	41426	0.0 %	41426				

LB107410 INSTRUMENT ID :CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Jan 2020 13:21:17

Sample ID	Extended ID	μ Abs	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	SD.0	125	-	0.00007470A	PPB	29 Jan 2020 14:37:51	S	Std
0.2 - 1	SD.2	1002	-	0.20007470A	PPB	29 Jan 2020 14:39:58	S	Std
2.5 - 1	SD.5	10376	-	2.50007470A	PPB	29 Jan 2020 14:42:06	S	Std
5.0 - 1	SD.5	20005	-	5.00007470A	PPB	29 Jan 2020 14:44:13	S	Std
7.5 - 1	SD.5	32174	-	7.50007470A	PPB	29 Jan 2020 14:53:19	S	Std
10.0 - 1	SD.5	41426	-	10.00007470A	PPB	29 Jan 2020 14:55:25	S	Std
ICV92 - 1	ICV92	16340	3.9175	-7470A	PPB	29 Jan 2020 15:10:00	U	SMPL
ICB92 - 1	ICB92	168	0.0391	-7470A	PPB	29 Jan 2020 15:12:05	U	SMPL
CCV34 - 1	CCV34	20076	4.8135	-7470A	PPB	29 Jan 2020 15:14:11	U	SMPL
CCB34 - 1	CCB34	175	0.0408	-7470A	PPB	29 Jan 2020 15:16:16	U	SMPL
CRA - 1	CRA	1000	0.2386	-7470A	PPB	29 Jan 2020 15:18:22	U	SMPL
HighStd - 1	HighStd	41234	9.8876	-7470A	PPB	29 Jan 2020 15:20:28	U	SMPL
ChkStd - 1	ChkStd	30210	7.2438	-7470A	PPB	29 Jan 2020 15:22:33	U	SMPL
PB126418BL - 1	PBW	183	0.0427	-7470A	PPB	29 Jan 2020 15:24:41	U	SMPL
PB126418BS - 1	LCSW	16554	3.9688	-7470A	PPB	29 Jan 2020 15:26:47	U	SMPL
L1190-04 - 1	TSP-02	1568	0.3749	-7470A	PPB	29 Jan 2020 15:28:54	U	SMPL
L1245-01 - 1	20200063-AMENDED-COMP-1	622	0.1480	-7470A	PPB	29 Jan 2020 15:31:01	U	SMPL
L1245-02 - 1	20200064-AMENDED-COMP-2	577	0.1372	-7470A	PPB	29 Jan 2020 15:33:09	U	SMPL
L1245-03 - 1	20200065-AMENDED-COMP-3	603	0.1434	-7470A	PPB	29 Jan 2020 15:35:17	U	SMPL
L1245-04 - 1	20200066-AMENDED-COMP-4	141	0.0326	-7470A	PPB	29 Jan 2020 15:37:22	U	SMPL
CCV35 - 1	CCV35	20267	4.8593	-7470A	PPB	29 Jan 2020 15:39:28	U	SMPL
CCB35 - 1	CCB35	134	0.0310	-7470A	PPB	29 Jan 2020 15:41:35	U	SMPL
L1245-05 - 1	20200067-AMENDED-COMP-5	799	0.1904	-7470A	PPB	29 Jan 2020 15:43:40	U	SMPL
L1245-05DUP - 1	20200067-AMENDED-COMP-5DUP	787	0.1876	-7470A	PPB	29 Jan 2020 15:45:47	U	SMPL
L1245-05MS - 1	20200067-AMENDED-COMP-5MS	18611	4.4621	-7470A	PPB	29 Jan 2020 15:47:53	U	SMPL
L1245-05MSD - 1	20200067-AMENDED-COMP-5MSD	18381	4.4070	-7470A	PPB	29 Jan 2020 15:49:59	U	SMPL
PB126419BL - 1	PBW	122	0.0281	-7470A	PPB	29 Jan 2020 15:52:06	U	SMPL
PB126419BS - 1	LCSW	16395	3.9307	-7470A	PPB	29 Jan 2020 15:54:13	U	SMPL
L1255-02 - 1	0072-FIELD-BLANK	56	0.0122	-7470A	PPB	29 Jan 2020 15:56:20	U	SMPL
L1255-03 - 1	0073-SITE-WATER	151	0.0350	-7470A	PPB	29 Jan 2020 15:58:28	U	SMPL
L1255-03DUP - 1	0073-SITE-WATERDUP	133	0.0307	-7470A	PPB	29 Jan 2020 16:00:35	U	SMPL
L1255-03MS - 1	0073-SITE-WATERMS	18994	4.5540	-7470A	PPB	29 Jan 2020 16:02:41	U	SMPL
CCV36 - 1	CCV36	20357	4.8809	-7470A	PPB	29 Jan 2020 16:10:45	U	SMPL
CCB36 - 1	CCB36	109	0.0250	-7470A	PPB	29 Jan 2020 16:12:51	U	SMPL
L1255-03MSD - 1	0073-SITE-WATERMSD	19061	4.5700	-7470A	PPB	29 Jan 2020 16:14:57	U	SMPL
L1264-01 - 1	CTY-GW-01-12	4613	1.1051	-7470A	PPB	29 Jan 2020 16:17:03	U	SMPL
L1265-01 - 1	CTY-WC-L-01	232	0.0545	-7470A	PPB	29 Jan 2020 16:19:09	U	SMPL
L1266-01 - 1	40652	140	0.0324	-7470A	PPB	29 Jan 2020 16:21:15	U	SMPL
L1008-21 - 1	CL-02-012420	130	0.0300	-7470A	PPB	29 Jan 2020 16:23:22	U	SMPL
L1008-21DUP - 1	CL-02-012420DUP	146	0.0338	-7470A	PPB	29 Jan 2020 16:25:29	U	SMPL
L1008-21MS - 1	CL-02-012420MS	16852	4.0403	-7470A	PPB	29 Jan 2020 16:27:35	U	SMPL
L1008-21MSD - 1	CL-02-012420MSD	16785	4.0242	-7470A	PPB	29 Jan 2020 16:29:43	U	SMPL
L1010-12 - 1	OK-01-012420	124	0.0286	-7470A	PPB	29 Jan 2020 16:31:51	U	SMPL
L1017-09 - 1	TR-04-012420	148	0.0343	-7470A	PPB	29 Jan 2020 16:33:57	U	SMPL
CCV37 - 1	CCV37	20565	4.9307	-7470A	PPB	29 Jan 2020 16:47:02	U	SMPL
CCB37 - 1	CCB37	142	0.0329	-7470A	PPB	29 Jan 2020 16:49:08	U	SMPL
L1262-02 - 1	B10(0-15)	124	0.0286	-7470A	PPB	29 Jan 2020 16:51:14	U	SMPL
L1265-02 - 1	CTY-WC-S-SB-0203	150	0.0348	-7470A	PPB	29 Jan 2020 16:53:20	U	SMPL
L1269-06 - 1	TP-22-21-COMP	134	0.0310	-7470A	PPB	29 Jan 2020 16:55:26	U	SMPL
L1269-14 - 1	TP-25-24-COMP	162	0.0377	-7470A	PPB	29 Jan 2020 16:57:32	U	SMPL
L1245-05LX5 - 1		190	0.0444	-7470A	PPB	29 Jan 2020 16:59:39	U	SMPL
L1255-03LX5 - 1		43	0.0091	-7470A	PPB	29 Jan 2020 17:01:46	U	SMPL
L1008-21LX5 - 1		55	0.0120	-7470A	PPB	29 Jan 2020 17:03:53	U	SMPL
PB126420BL - 1	PBW	121	0.0278	-7470A	PPB	29 Jan 2020 17:06:01	U	SMPL
PB126420BS - 1	LCSW	16551	3.9681	-7470A	PPB	29 Jan 2020 17:08:08	U	SMPL
PB126420TB - 1	PB126348TB	133	0.0307	-7470A	PPB	29 Jan 2020 17:10:14	U	SMPL
CCV38 - 1	CCV38	20246	4.8542	-7470A	PPB	29 Jan 2020 17:12:21	U	SMPL
CCB38 - 1	CCB38	118	0.0271	-7470A	PPB	29 Jan 2020 17:14:27	U	SMPL
PB126418TB - 1	PB126338TB	139	0.0322	-7470A	PPB	29 Jan 2020 17:16:33	U	SMPL
CCV39 - 1	CCV39	20651	4.9514	-7470A	PPB	29 Jan 2020 17:18:39	U	SMPL
CCB39 - 1	CCB39	-33	-0.0091	-7470A	PPB	29 Jan 2020 17:20:45	U	SMPL