


LB 107578

245.1

INSTRUMENT ID: 9X1

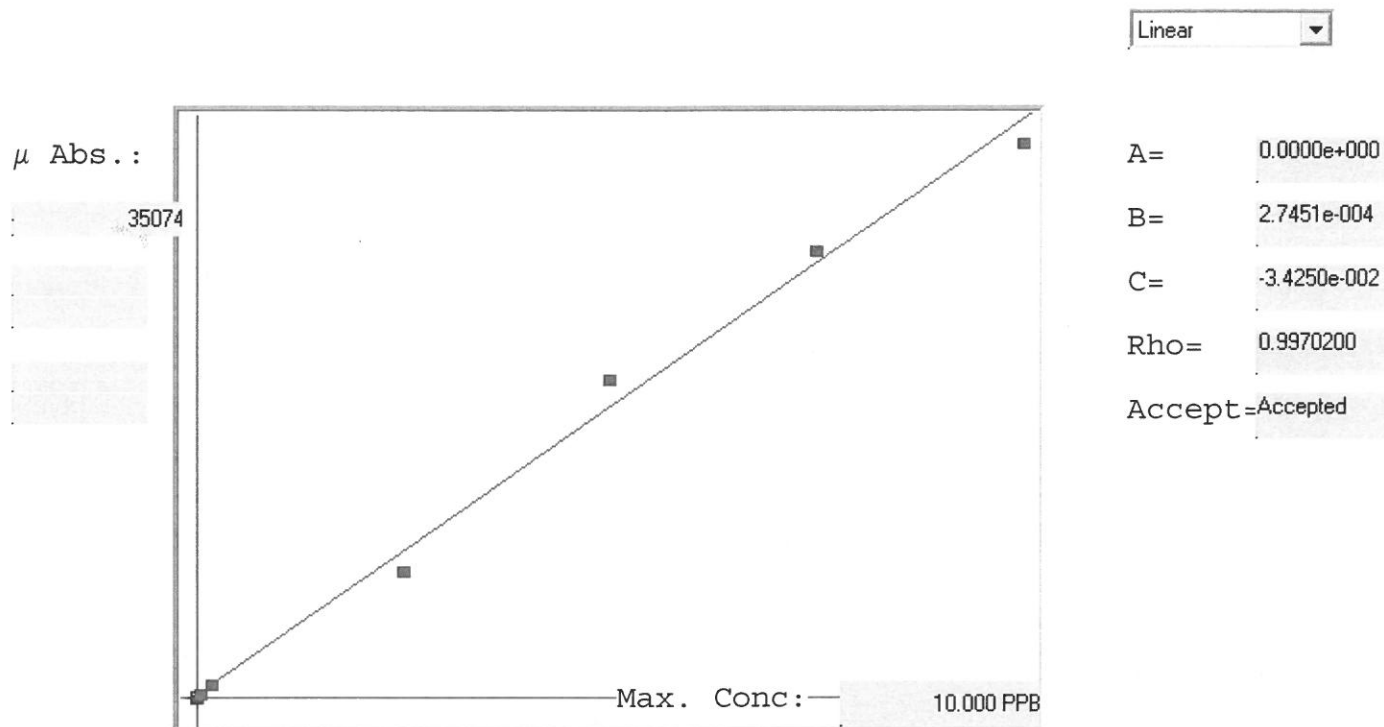

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	45	0.000	45				
0.05	0.050	0.045	-0.005	288	0.0 %	288				
0.2	0.200	0.211	0.011	895	0.0 %	895				
2.5	2.500	2.184	-0.316	8080	0.0 %	8080				
5.0	5.000	5.504	0.504	20174	0.0 %	20174				
7.5	7.500	7.734	0.234	28299	0.0 %	28299				
10.0	10.000	9.594	-0.406	35074	0.0 %	35074				

LB107578 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 06 Feb 2020 10:52:33

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	45	-	0.0000	245.1	PPB	06 Feb 2020 13:33:06	S	Std
0.05 - 1	SO.05	288	-	0.0500	245.1	PPB	06 Feb 2020 13:35:23	S	Std
0.2 - 1	SO.2	895	-	0.2000	245.1	PPB	06 Feb 2020 13:37:39	S	Std
2.5 - 1	SO.25	8080	-	2.5000	245.1	PPB	06 Feb 2020 13:39:56	S	Std
5.0 - 1	SE	20174	-	5.0000	245.1	PPB	06 Feb 2020 13:42:12	S	Std
7.5 - 1	SE.5	28299	-	7.5000	245.1	PPB	06 Feb 2020 13:44:28	S	Std
10.0 - 1	SIJ	35074	-	10.0000	245.1	PPB	06 Feb 2020 13:52:10	S	Std
ICV03 - 1	ICV03	14760	4.0175	-245.1		PPB	06 Feb 2020 13:55:11	U	SMPL
ICB03 - 1	ICB03	41	-0.0230	-245.1		PPB	06 Feb 2020 13:57:25	U	SMPL
CCV77 - 1	CCV77	19653	5.3607	-245.1		PPB	06 Feb 2020 13:59:40	U	SMPL
CCB77 - 1	CCB77	36	-0.0244	-245.1		PPB	06 Feb 2020 14:01:55	U	SMPL
CRA - 1	CRA	263	0.0379	-245.1		PPB	06 Feb 2020 14:04:10	U	SMPL
HighStd - 1	HighStd	34736	9.5012	-245.1		PPB	06 Feb 2020 14:06:25	U	SMPL
ChkStd - 1	ChkStd	28292	7.7322	-245.1		PPB	06 Feb 2020 14:08:40	U	SMPL
PB126619BL - 1	PBW	17	-0.0296	-245.1		PPB	06 Feb 2020 14:10:56	U	SMPL
PB126619BS - 1	LCSW	16190	4.4101	-245.1		PPB	06 Feb 2020 14:13:12	U	SMPL
L1332-01 - 1	KIT-SINK-1ST-DRAW	94	-0.0084	-245.1		PPB	06 Feb 2020 14:15:29	U	SMPL
L1377-01 - 1	BW-2	200	0.0207	-245.1		PPB	06 Feb 2020 14:17:44	U	SMPL
L1377-01DUP - 1	BW-2DUP	-14	-0.0381	-245.1		PPB	06 Feb 2020 14:20:01	U	SMPL
L1377-02 - 1	L1377-01MS	16701	4.5504	-245.1		PPB	06 Feb 2020 14:22:18	U	SMPL
L1377-03 - 1	L1377-01MSD	16958	4.6209	-245.1		PPB	06 Feb 2020 14:24:33	U	SMPL
CCV78 - 1	CCV78	17800	4.8521	-245.1		PPB	06 Feb 2020 14:26:49	U	SMPL
CCB78 - 1	CCB78	42	-0.0227	-245.1		PPB	06 Feb 2020 14:29:04	U	SMPL
L1377-04 - 1	FB-02032020	-86	-0.0579	-245.1		PPB	06 Feb 2020 14:31:20	U	SMPL
L1377-05 - 1	BW-209	287	0.0445	-245.1		PPB	06 Feb 2020 14:33:35	U	SMPL
L1407-02 - 1	COMP	272	0.0404	-245.1		PPB	06 Feb 2020 14:35:51	U	SMPL
L1377-01LX5 - 1		34	-0.0249	-245.1		PPB	06 Feb 2020 14:41:31	U	SMPL
L1377-01A - 1		16835	4.5871	-245.1		PPB	06 Feb 2020 14:43:46	U	SMPL
CCV79 - 1	CCV79	17864	4.8696	-245.1		PPB	06 Feb 2020 14:46:02	U	SMPL
CCB79 - 1	CCB79	9	-0.0318	-245.1		PPB	06 Feb 2020 14:48:19	U	SMPL