


LB 107594

7471B

INSTRUMENT ID: CV1

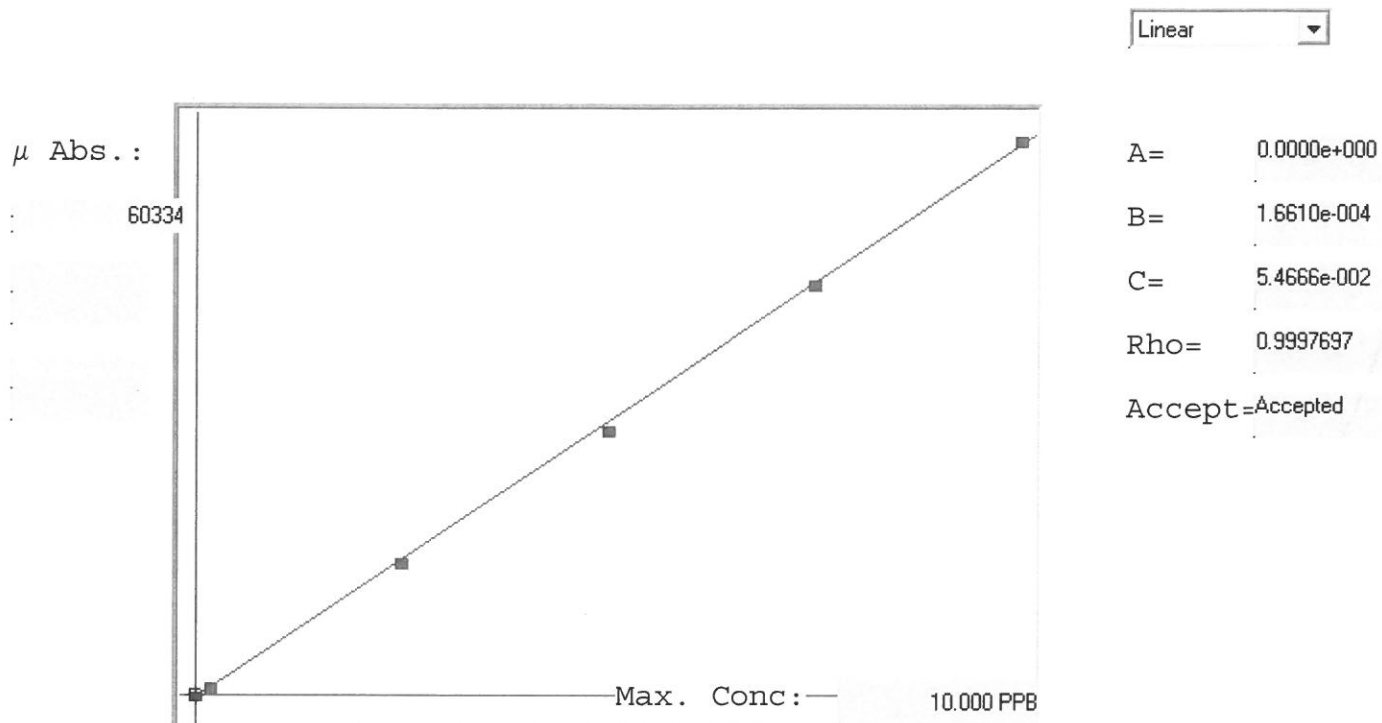

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.077	0.077	135	0.000	135				
0.2	0.200	0.223	0.023	1013	0.0 %	1013				
2.5	2.500	2.475	-0.025	14572	0.0 %	14572				
5.0	5.000	4.843	-0.157	28827	0.0 %	28827				
7.5	7.500	7.506	0.006	44858	0.0 %	44858				
10.0	10.000	10.076	0.076	60334	0.0 %	60334				

LB107594 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 06 Feb 2020 15:13:06					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	135	-	0.0000	7471B	PPB	06 Feb 2020 15:15:23	S	Std
0.2 - 1	50.2	1013	-	0.2000	7471B	PPB	06 Feb 2020 15:17:40	S	Std
2.5 - 1	52.5	14572	-	2.5000	7471B	PPB	06 Feb 2020 15:19:57	S	Std
5.0 - 1	55	28827	-	5.0000	7471B	PPB	06 Feb 2020 15:22:14	S	Std
7.5 - 1	57.5	44858	-	7.5000	7471B	PPB	06 Feb 2020 15:24:31	S	Std
10.0 - 1	510	60334	-	10.0000	7471B	PPB	06 Feb 2020 15:32:59	S	Std
ICV04 - 1	ICV04	22154	3.7345	-	7471B	PPB	06 Feb 2020 15:35:44	U	SMPL
ICB04 - 1	ICB04	24	0.0587	-	7471B	PPB	06 Feb 2020 15:37:59	U	SMPL
CCV80 - 1	CCV80	29137	4.8944	-	7471B	PPB	06 Feb 2020 15:40:14	U	SMPL
CCB80 - 1	CCB80	31	0.0598	-	7471B	PPB	06 Feb 2020 15:42:29	U	SMPL
CRA - 1	CRA	974	0.2164	-	7471B	PPB	06 Feb 2020 15:44:43	U	SMPL
HighStd - 1	HighStd	60708	10.1384	-	7471B	PPB	06 Feb 2020 15:46:58	U	SMPL
ChkStd - 1	ChkStd	42049	7.0391	-	7471B	PPB	06 Feb 2020 15:49:14	U	SMPL
PB126616BL - 1	PBS	60	0.0646	-	7471B	PPB	06 Feb 2020 15:51:30	U	SMPL
PB126616BS - 1	LCSS	22219	3.7453	-	7471B	PPB	06 Feb 2020 15:53:46	U	SMPL
L1347-02 - 1	COMP-01	7898	1.3665	-	7471B	PPB	06 Feb 2020 15:56:02	U	SMPL
L1347-02DUP - 1	COMP-01DUP	7158	1.2436	-	7471B	PPB	06 Feb 2020 15:58:18	U	SMPL
L1347-02MS - 1	COMP-01MS	30543	5.1279	-	7471B	PPB	06 Feb 2020 16:03:10	U	SMPL
L1347-02MSD - 1	COMP-01MSD	30888	5.1852	-	7471B	PPB	06 Feb 2020 16:05:27	U	SMPL
L1351-01 - 1	TAL-1	6795	1.1833	-	7471B	PPB	06 Feb 2020 16:07:41	U	SMPL
CCV81 - 1	CCV81	29008	4.8730	-	7471B	PPB	06 Feb 2020 16:09:56	U	SMPL
CCB81 - 1	CCB81	26	0.0590	-	7471B	PPB	06 Feb 2020 16:12:11	U	SMPL
L1351-02 - 1	TAL-2	6160	1.0779	-	7471B	PPB	06 Feb 2020 16:14:27	U	SMPL
L1351-03 - 1	TAL-3	7138	1.2403	-	7471B	PPB	06 Feb 2020 16:16:42	U	SMPL
L1363-01 - 1	HR-06-020320	4087	0.7335	-	7471B	PPB	06 Feb 2020 16:18:58	U	SMPL
L1383-01 - 1	TP-A	277220	46.1016	-	7471B	PPB	06 Feb 2020 16:21:13	U	SMPL
L1383-05 - 1	TP-B	6239	1.0910	-	7471B	PPB	06 Feb 2020 16:23:29	U	SMPL
L1383-09 - 1	TP-C	44534	7.4519	-	7471B	PPB	06 Feb 2020 16:25:47	U	SMPL
L1390-01 - 1	SB-1	582	0.1513	-	7471B	PPB	06 Feb 2020 16:28:04	U	SMPL
L1390-02 - 1	SB-2	261	0.0980	-	7471B	PPB	06 Feb 2020 16:30:21	U	SMPL
L1390-03 - 1	SB-3	510	0.1394	-	7471B	PPB	06 Feb 2020 16:32:38	U	SMPL
L1390-04 - 1	SB-4	1014	0.2231	-	7471B	PPB	06 Feb 2020 16:34:53	U	SMPL
CCV82 - 1	CCV82	29963	5.0316	-	7471B	PPB	06 Feb 2020 16:37:09	U	SMPL
CCB82 - 1	CCB82	73	0.0668	-	7471B	PPB	06 Feb 2020 16:39:24	U	SMPL
L1390-05 - 1	SB-5	194952	32.4367	-	7471B	PPB	06 Feb 2020 16:41:40	U	SMPL
PB126621BL - 1	PBS	268	0.0992	-	7471B	PPB	06 Feb 2020 16:43:55	U	SMPL
PB126621BS - 1	LCSS	22633	3.8141	-	7471B	PPB	06 Feb 2020 16:46:13	U	SMPL
L1365-01 - 1	CL-01-020520	1995	0.3860	-	7471B	PPB	06 Feb 2020 16:48:29	U	SMPL
L1365-01DUP - 1	CL-01-020520DUP	2030	0.3919	-	7471B	PPB	06 Feb 2020 16:50:44	U	SMPL
L1365-01MS - 1	CL-01-020520MS	24297	4.0905	-	7471B	PPB	06 Feb 2020 16:58:10	U	SMPL
L1365-01MSD - 1	CL-01-020520MSD	25290	4.2554	-	7471B	PPB	06 Feb 2020 17:00:26	U	SMPL
L1394-08 - 1	MNR-WHITE-PLAINS-COMP	279	0.1010	-	7471B	PPB	06 Feb 2020 17:02:43	U	SMPL
L1408-01 - 1	SHORE-RD-PATH-BH-01-A	20862	3.5199	-	7471B	PPB	06 Feb 2020 17:05:00	U	SMPL
L1408-02 - 1	SHORE-RD-PATH-BH-01-B	1294	0.2696	-	7471B	PPB	06 Feb 2020 17:07:15	U	SMPL
CCV83 - 1	CCV83	31098	5.2201	-	7471B	PPB	06 Feb 2020 17:09:31	U	SMPL
CCB83 - 1	CCB83	113	0.0734	-	7471B	PPB	06 Feb 2020 17:14:35	U	SMPL
L1408-05 - 1	SHORE-RD-PATH-BH-03-A	41639	6.9710	-	7471B	PPB	06 Feb 2020 17:16:50	U	SMPL
L1408-06 - 1	SHORE-RD-PATH-BH-03-B	23777	4.0041	-	7471B	PPB	06 Feb 2020 17:19:05	U	SMPL
L1408-09 - 1	SHORE-RD-PATH-BH-02-A	9153	1.5750	-	7471B	PPB	06 Feb 2020 17:21:20	U	SMPL
L1408-10 - 1	SHORE-RD-PATH-BH-02-B	10725	1.8361	-	7471B	PPB	06 Feb 2020 17:23:35	U	SMPL
L1408-11 - 1	SHORE-RD-PATH-BH-04-A	322783	HIGH	-	7471B	PPB	06 Feb 2020 17:25:51	X	
L1408-12 - 1	SHORE-RD-PATH-BH-04-B	8631	1.4883	-	7471B	PPB	06 Feb 2020 17:27:42	U	SMPL
L1409-01 - 1	ROW-6-5	16887	2.8596	-	7471B	PPB	06 Feb 2020 17:30:00	U	SMPL
CCV84 - 1	CCV84	30286	5.0852	-	7471B	PPB	06 Feb 2020 17:32:17	U	SMPL
CCB84 - 1	CCB84	-51	0.0462	-	7471B	PPB	06 Feb 2020 17:34:34	U	SMPL
L1408-11DLX10 - 1		40474	6.7775	-	7471B	PPB	06 Feb 2020 17:36:50	U	SMPL
L1347-02LX5 - 1		1685	0.3345	-	7471B	PPB	06 Feb 2020 17:39:05	U	SMPL
L1347-02A - 1		32716	5.4889	-	7471B	PPB	06 Feb 2020 17:41:21	U	SMPL
L1365-01LX5 - 1		619	0.1575	-	7471B	PPB	06 Feb 2020 17:43:37	U	SMPL
L1365-01A - 1		24777	4.1702	-	7471B	PPB	06 Feb 2020 17:48:34	U	SMPL
L1383-01DLX10 - 1		29754	4.9969	-	7471B	PPB	06 Feb 2020 17:50:50	U	SMPL
L1390-05DLX5 - 1		34498	5.7849	-	7471B	PPB	06 Feb 2020 17:53:05	U	SMPL
CCV85 - 1	CCV85	30475	5.1166	-	7471B	PPB	06 Feb 2020 17:55:20	U	SMPL
CCB85 - 1	CCB85	-35	0.0489	-	7471B	PPB	06 Feb 2020 17:57:38	U	SMPL