


LB107668

7470A

INSTRUMENT ID: CY1

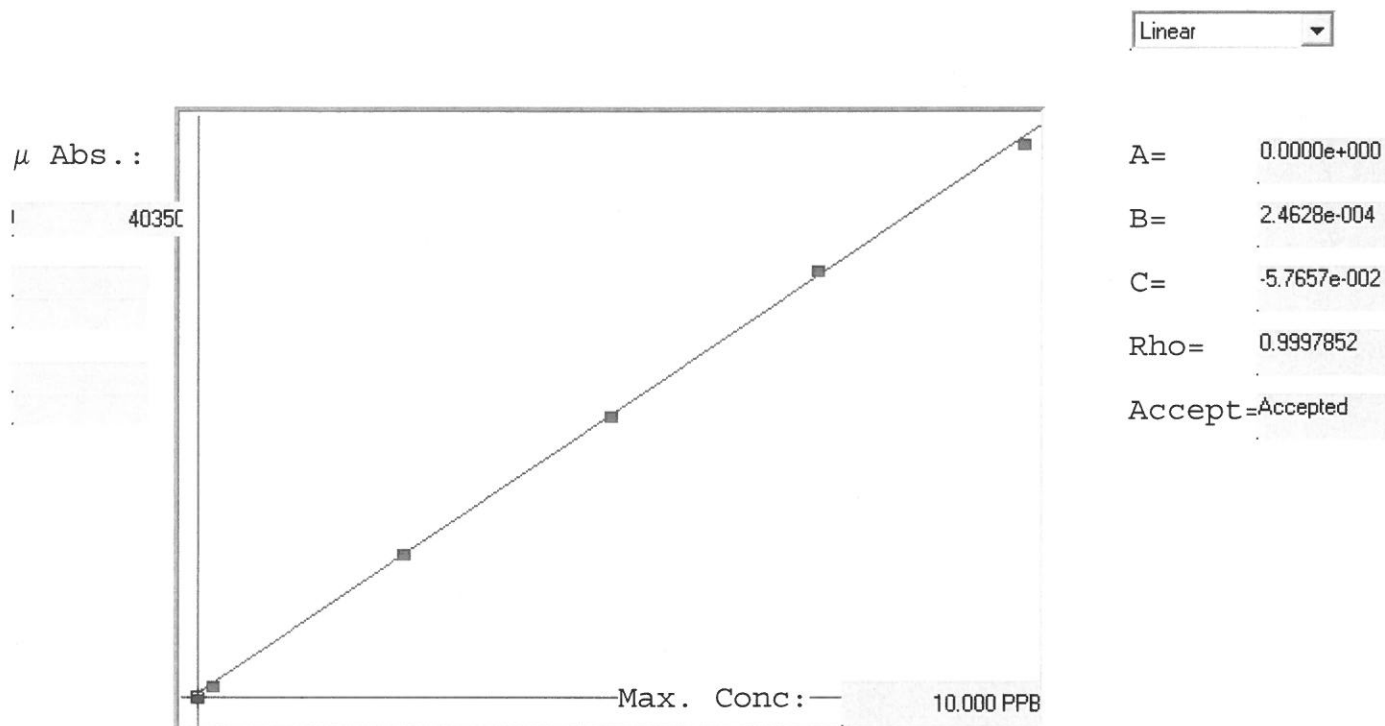

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.051	-0.051	28	0.000	28				
0.2	0.200	0.181	-0.019	970	0.0 %	970				
2.5	2.500	2.536	0.036	10532	0.0 %	10532				
5.0	5.000	5.029	0.029	20652	0.0 %	20652				
7.5	7.500	7.625	0.125	31194	0.0 %	31194				
10.0	10.000	9.880	-0.120	40350	0.0 %	40350				

LB107663 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 10 Feb 2020 10:23:30						
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date		Type	Type
0.0 - 1	50	28	-	0.0000	7470A	PPB	10 Feb 2020	10:38:31	S	Std
0.2 - 1	50.2	970	-	0.2000	7470A	PPB	10 Feb 2020	10:40:38	S	Std
2.5 - 1	52.5	10532	-	2.5000	7470A	PPB	10 Feb 2020	10:42:45	S	Std
5.0 - 1	55	20652	-	5.0000	7470A	PPB	10 Feb 2020	10:44:53	S	Std
7.5 - 1	57.5	31194	-	7.5000	7470A	PPB	10 Feb 2020	10:47:00	S	Std
10.0 - 1	510	40350	-	10.0000	7470A	PPB	10 Feb 2020	10:49:06	S	Std
ICV08 - 1	ICV08	15858	3.8479		-7470A	PPB	10 Feb 2020	10:52:59	U	SMPL
ICB08 - 1	ICB08	0	-0.0577		-7470A	PPB	10 Feb 2020	10:55:04	U	SMPL
CCV95 - 1	CCV95	21719	5.2914		-7470A	PPB	10 Feb 2020	10:57:10	U	SMPL
CCB95 - 1	CCB95	0	-0.0577		-7470A	PPB	10 Feb 2020	10:59:15	U	SMPL
CRA - 1	CRA	956	0.1778		-7470A	PPB	10 Feb 2020	11:01:21	U	SMPL
HighStd - 1	HighStd	40613	9.9446		-7470A	PPB	10 Feb 2020	11:03:26	U	SMPL
ChkStd - 1	ChkStd	29351	7.1710		-7470A	PPB	10 Feb 2020	11:05:32	U	SMPL
PB126685BL - 1	PBW	-17	-0.0618		-7470A	PPB	10 Feb 2020	11:07:38	U	SMPL
PB126685BS - 1	LCSW	16371	3.9742		-7470A	PPB	10 Feb 2020	11:09:45	U	SMPL
L1419-02 - 1	30576	906	0.1655		-7470A	PPB	10 Feb 2020	11:11:52	U	SMPL
L1419-03 - 1	COMP-1	197	-0.0091		-7470A	PPB	10 Feb 2020	11:13:59	U	SMPL
L1419-08 - 1	51067	278	0.0108		-7470A	PPB	10 Feb 2020	11:16:07	U	SMPL
L1430-01 - 1	N29305	16	-0.0537		-7470A	PPB	10 Feb 2020	11:18:14	U	SMPL
L1430-01DUP - 1	N29305DUP	4	-0.0567		-7470A	PPB	10 Feb 2020	11:20:20	U	SMPL
CCV96 - 1	CCV96	21656	5.2758		-7470A	PPB	10 Feb 2020	11:22:26	U	SMPL
CCB96 - 1	CCB96	-4	-0.0586		-7470A	PPB	10 Feb 2020	11:24:31	U	SMPL
L1430-01MS - 1	N29305MS	17638	4.2863		-7470A	PPB	10 Feb 2020	11:26:37	U	SMPL
L1430-01MSD - 1	N29305MSD	17076	4.1479		-7470A	PPB	10 Feb 2020	11:28:43	U	SMPL
L1432-08 - 1	OD-COMP	446	0.0522		-7470A	PPB	10 Feb 2020	11:30:49	U	SMPL
L1432-10 - 1	40276	322	0.0216		-7470A	PPB	10 Feb 2020	11:32:55	U	SMPL
L1437-02 - 1	GROUNDWATER	50	-0.0453		-7470A	PPB	10 Feb 2020	11:35:02	U	SMPL
PB126686BL - 1	PB126686BL	-11	-0.0604		-7470A	PPB	10 Feb 2020	11:37:09	U	SMPL
PB126686BS - 1	PB126686BS	16026	3.8893		-7470A	PPB	10 Feb 2020	11:39:16	U	SMPL
L1431-03 - 1	VNJ-209	-15	-0.0614		-7470A	PPB	10 Feb 2020	11:41:24	U	SMPL
L1431-06 - 1	350	8	-0.0557		-7470A	PPB	10 Feb 2020	11:43:31	U	SMPL
L1431-09 - 1	06	16	-0.0537		-7470A	PPB	10 Feb 2020	11:45:38	U	SMPL
CCV97 - 1	CCV97	21872	5.3290		-7470A	PPB	10 Feb 2020	11:47:44	U	SMPL
CCB97 - 1	CCB97	-7	-0.0594		-7470A	PPB	10 Feb 2020	11:49:50	U	SMPL
L1431-12 - 1	72-11986	12	-0.0547		-7470A	PPB	10 Feb 2020	11:51:56	U	SMPL
L1433-02 - 1	349	10	-0.0552		-7470A	PPB	10 Feb 2020	11:54:02	U	SMPL
L1433-02DUP - 1	349DUP	13	-0.0545		-7470A	PPB	10 Feb 2020	11:56:08	U	SMPL
L1433-02MS - 1	349MS	15811	3.8363		-7470A	PPB	10 Feb 2020	11:58:14	U	SMPL
L1433-02MSD - 1	349MSD	16559	4.0205		-7470A	PPB	10 Feb 2020	12:00:21	U	SMPL
L1430-01LX5 - 1		-4	-0.0586		-7470A	PPB	10 Feb 2020	12:02:28	U	SMPL
L1430-01A - 1		18434	4.4823		-7470A	PPB	10 Feb 2020	12:04:35	U	SMPL
L1433-02LX5 - 1		6	-0.0562		-7470A	PPB	10 Feb 2020	12:06:42	U	SMPL
L1433-02A - 1		17104	4.1548		-7470A	PPB	10 Feb 2020	12:08:49	U	SMPL
PB126686TB - 1	PB126639TB	-8	-0.0596		-7470A	PPB	10 Feb 2020	12:10:56	U	SMPL
CCV98 - 1	CCV98	21983	5.3564		-7470A	PPB	10 Feb 2020	12:13:02	U	SMPL
CCB98 - 1	CCB98	-13	-0.0609		-7470A	PPB	10 Feb 2020	12:15:08	U	SMPL