


LB 107696

7471B

INSTRUMENT ID: CV1

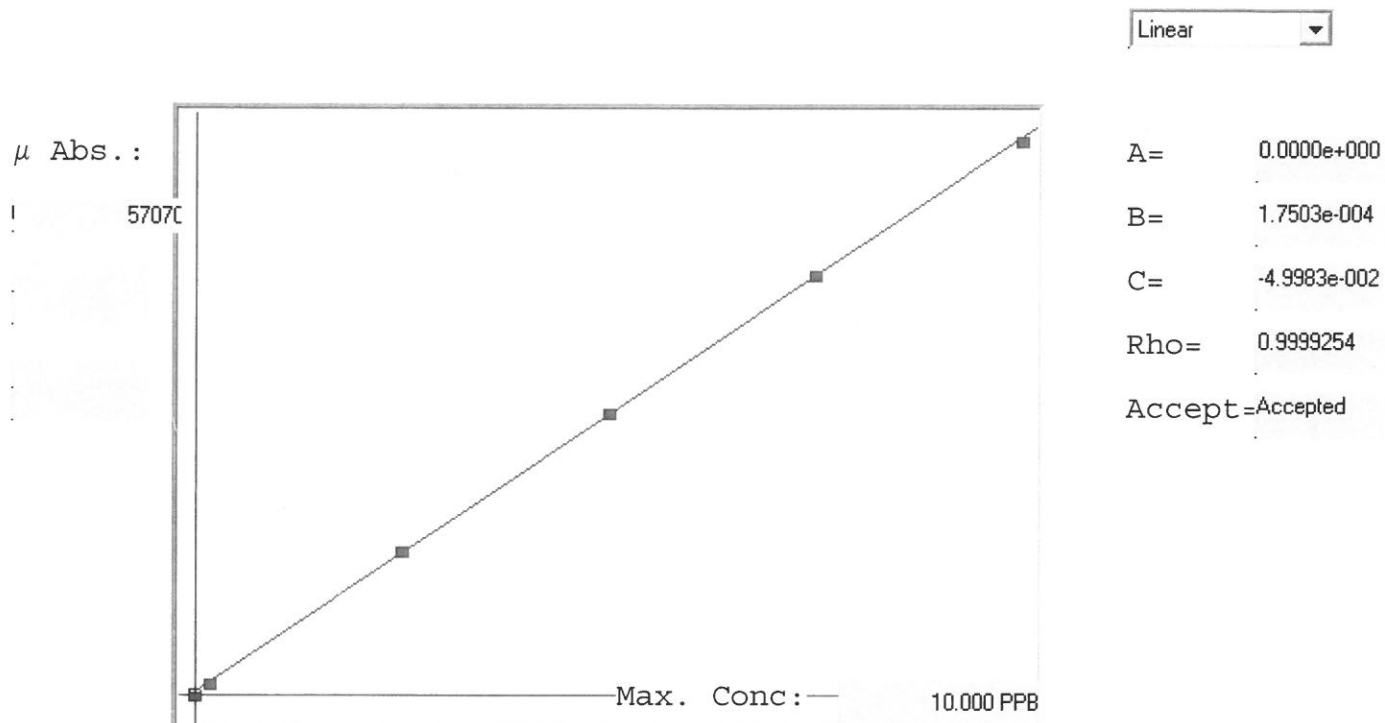

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.048	-0.048	10	0.000	10				
0.2	0.200	0.180	-0.020	1313	0.0 %	1313				
2.5	2.500	2.550	0.050	14855	0.0 %	14855				
5.0	5.000	5.047	0.047	29122	0.0 %	29122				
7.5	7.500	7.532	0.032	43315	0.0 %	43315				
10.0	10.000	9.939	-0.061	57070	0.0 %	57070				

LB107696 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 Feb 2020 13:54:21

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	10	-	0.00007471B	PPB		11 Feb 2020 13:56:39	S	Std
0.2 - 1	50.2	1313	-	0.20007471B	PPB		11 Feb 2020 13:58:56	S	Std
2.5 - 1	52.5	14855	-	2.50007471B	PPB		11 Feb 2020 14:01:12	S	Std
5.0 - 1	55	29122	-	5.00007471B	PPB		11 Feb 2020 14:03:29	S	Std
7.5 - 1	57.5	43315	-	7.50007471B	PPB		11 Feb 2020 14:05:45	S	Std
10.0 - 1	510	57070	-	10.00007471B	PPB		11 Feb 2020 14:08:01	S	Std
ICV11 - 1	ICV11	21814	3.7682	-7471B	PPB		11 Feb 2020 14:10:45	U	SMPL
ICB11 - 1	ICB11	-28	-0.0549	-7471B	PPB		11 Feb 2020 14:12:59	U	SMPL
CCV09 - 1	CCV09	29313	5.0808	-7471B	PPB		11 Feb 2020 14:15:14	U	SMPL
CCB09 - 1	CCB09	-27	-0.0547	-7471B	PPB		11 Feb 2020 14:17:29	U	SMPL
CRA - 1	CRA	1302	0.1779	-7471B	PPB		11 Feb 2020 14:19:44	U	SMPL
HighStd - 1	HighStd	57535	10.0206	-7471B	PPB		11 Feb 2020 14:21:59	U	SMPL
ChkStd - 1	ChkStd	39727	6.9036	-7471B	PPB		11 Feb 2020 14:24:14	U	SMPL
PB126728BL - 1	PBS	-64	-0.0612	-7471B	PPB		11 Feb 2020 14:26:30	U	SMPL
PB126728BS - 1	LCSS	21843	3.7733	-7471B	PPB		11 Feb 2020 14:28:47	U	SMPL
L1452-01 - 1	SPARTA-TSB	2846	0.4482	-7471B	PPB		11 Feb 2020 14:31:03	U	SMPL
L1452-01DUP - 1	SPARTA-TSBDUP	2814	0.4426	-7471B	PPB		11 Feb 2020 14:33:20	U	SMPL
L1452-01MS - 1	SPARTA-TSBMS	24437	4.2273	-7471B	PPB		11 Feb 2020 14:35:36	U	SMPL
L1452-01MSD - 1	SPARTA-TSBMSD	24375	4.2165	-7471B	PPB		11 Feb 2020 14:37:53	U	SMPL
L1456-04 - 1	ETGI-337-290	3617	0.5831	-7471B	PPB		11 Feb 2020 14:40:09	U	SMPL
CCV10 - 1	CCV10	29395	5.0952	-7471B	PPB		11 Feb 2020 14:42:24	U	SMPL
CCB10 - 1	CCB10	-29	-0.0551	-7471B	PPB		11 Feb 2020 14:44:39	U	SMPL
L1468-01 - 1	TP11-EP1-2.5	3184	0.5073	-7471B	PPB		11 Feb 2020 14:46:55	U	SMPL
L1468-02 - 1	TP11-EP2-3	6062	1.0111	-7471B	PPB		11 Feb 2020 14:49:09	U	SMPL
L1468-03 - 1	TP10-EP1-2.5	15649	2.6891	-7471B	PPB		11 Feb 2020 14:51:25	U	SMPL
L1468-04 - 1	TP10-EP2-3	14869	2.5526	-7471B	PPB		11 Feb 2020 14:53:41	U	SMPL
L1468-05 - 1	TP9-EP1-2.5	48783	8.4887	-7471B	PPB		11 Feb 2020 14:55:57	U	SMPL
L1468-06 - 1	TP9-EP2-3	4223	0.6892	-7471B	PPB		11 Feb 2020 14:58:13	U	SMPL
L1473-01 - 1	P-1	929	0.1126	-7471B	PPB		11 Feb 2020 15:00:30	U	SMPL
L1452-01LX5 - 1		562	0.0484	-7471B	PPB		11 Feb 2020 15:02:46	U	SMPL
L1452-01A - 1		23365	4.0397	-7471B	PPB		11 Feb 2020 15:05:04	U	SMPL
CCV11 - 1	CCV11	29484	5.1107	-7471B	PPB		11 Feb 2020 15:07:19	U	SMPL
CCB11 - 1	CCB11	-24	-0.0542	-7471B	PPB		11 Feb 2020 15:09:34	U	SMPL