


LB 107712

7470A

INSTRUMENT ID : CV1

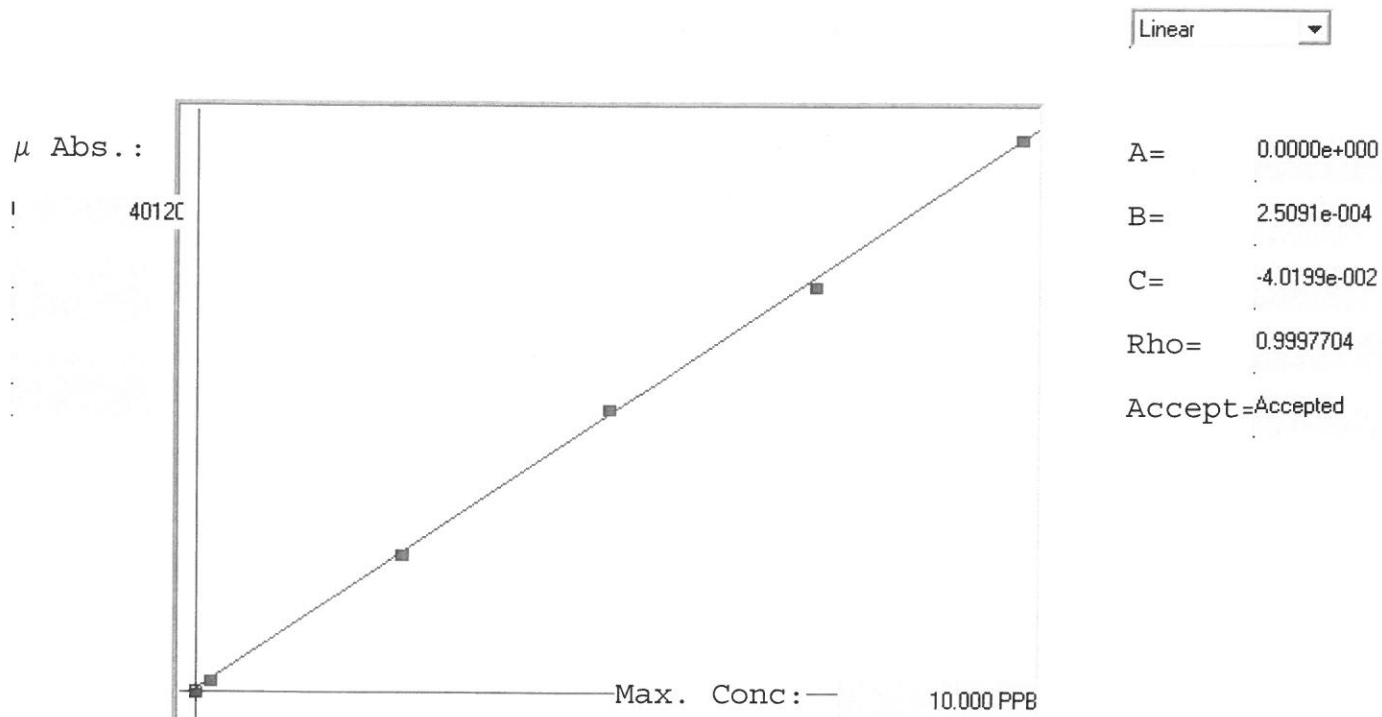

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.015	-0.015	102	0.000	102				
0.2	0.200	0.194	-0.006	935	0.0 %	935				
2.5	2.500	2.480	-0.020	10045	0.0 %	10045				
5.0	5.000	5.141	0.141	20650	0.0 %	20650				
7.5	7.500	7.372	-0.128	29543	0.0 %	29543				
10.0	10.000	10.026	0.026	40120	0.0 %	40120				

LB107712 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Feb 2020 09:58:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	102	-	0.0000	7470A	PPB	12 Feb 2020 10:00:31	S	Std
0.2 - 1	SD.2	935	-	0.2000	7470A	PPB	12 Feb 2020 10:02:38	S	Std
2.5 - 1	SD.5	10045	-	2.5000	7470A	PPB	12 Feb 2020 10:04:46	S	Std
5.0 - 1	SD.5	20650	-	5.0000	7470A	PPB	12 Feb 2020 10:06:53	S	Std
7.5 - 1	SD.5	29543	-	7.5000	7470A	PPB	12 Feb 2020 10:09:00	S	Std
10.0 - 1	SD.5	40120	-	10.0000	7470A	PPB	12 Feb 2020 10:11:06	S	Std
ICV12 - 1	ICV12	16229	4.0318	-	7470A	PPB	12 Feb 2020 10:13:37	U	SMPL
ICB12 - 1	ICB12	5	-0.0389	-	7470A	PPB	12 Feb 2020 10:15:42	U	SMPL
CCV12 - 1	CCV12	21224	5.2852	-	7470A	PPB	12 Feb 2020 10:17:48	U	SMPL
CCB12 - 1	CCB12	23	-0.0344	-	7470A	PPB	12 Feb 2020 10:19:53	U	SMPL
CRA - 1	CRA	933	0.1939	-	7470A	PPB	12 Feb 2020 10:21:59	U	SMPL
HighStd - 1	HighStd	40006	9.9978	-	7470A	PPB	12 Feb 2020 10:24:04	U	SMPL
ChkStd - 1	ChkStd	29041	7.2465	-	7470A	PPB	12 Feb 2020 10:26:10	U	SMPL
PB126719BL - 1	PBW	-38	-0.0497	-	7470A	PPB	12 Feb 2020 10:28:16	U	SMPL
PB126719BS - 1	LCSW	15371	3.8166	-	7470A	PPB	12 Feb 2020 10:30:23	U	SMPL
L1015-01 - 1	PR-MANHOLE	1359	0.3008	-	7470A	PPB	12 Feb 2020 10:32:30	U	SMPL
L1454-10 - 1	INK-PIT	558	0.0998	-	7470A	PPB	12 Feb 2020 10:34:37	U	SMPL
L1454-11 - 1	INK-TOTE	415	0.0639	-	7470A	PPB	12 Feb 2020 10:36:45	U	SMPL
L1456-01 - 1	FM-5213	8169	2.0095	-	7470A	PPB	12 Feb 2020 10:38:52	U	SMPL
L1456-01DUP - 1	FM-5213DUP	8168	2.0092	-	7470A	PPB	12 Feb 2020 10:40:59	U	SMPL
CCV13 - 1	CCV13	21343	5.3150	-	7470A	PPB	12 Feb 2020 10:43:04	U	SMPL
CCB13 - 1	CCB13	46	-0.0287	-	7470A	PPB	12 Feb 2020 10:45:10	U	SMPL
L1456-01MS - 1	FM-5213MS	24737	6.1666	-	7470A	PPB	12 Feb 2020 10:47:16	U	SMPL
L1456-01MSD - 1	FM-5213MSD	24965	6.2238	-	7470A	PPB	12 Feb 2020 10:49:22	U	SMPL
PB126754BL - 1	PBW	-32	-0.0482	-	7470A	PPB	12 Feb 2020 10:51:28	U	SMPL
PB126754BS - 1	LCSW	15196	3.7727	-	7470A	PPB	12 Feb 2020 10:53:34	U	SMPL
L1367-04 - 1	OK-03-021020	0	-0.0402	-	7470A	PPB	12 Feb 2020 10:55:41	U	SMPL
L1367-04DUP - 1	OK-03-021020DUP	14	-0.0367	-	7470A	PPB	12 Feb 2020 10:57:48	U	SMPL
L1367-04MS - 1	OK-03-021020MS	15305	3.8000	-	7470A	PPB	12 Feb 2020 10:59:55	U	SMPL
L1367-04MSD - 1	OK-03-021020MSD	14497	3.5973	-	7470A	PPB	12 Feb 2020 11:02:03	U	SMPL
L1372-05 - 1	SU-01-021020	14	-0.0367	-	7470A	PPB	12 Feb 2020 11:04:11	U	SMPL
L1373-03 - 1	TR-05-021020	22	-0.0347	-	7470A	PPB	12 Feb 2020 11:06:17	U	SMPL
CCV14 - 1	CCV14	21378	5.3238	-	7470A	PPB	12 Feb 2020 11:08:23	U	SMPL
CCB14 - 1	CCB14	37	-0.0309	-	7470A	PPB	12 Feb 2020 11:10:29	U	SMPL
L1475-01 - 1	02-10-A	23	-0.0344	-	7470A	PPB	12 Feb 2020 11:12:35	U	SMPL
L1475-02 - 1	02-10-B	30	-0.0327	-	7470A	PPB	12 Feb 2020 11:14:42	U	SMPL
L1475-03 - 1	02-10-C	23	-0.0344	-	7470A	PPB	12 Feb 2020 11:16:48	U	SMPL
L1475-04 - 1	02-10-D	32	-0.0322	-	7470A	PPB	12 Feb 2020 11:18:54	U	SMPL
L1475-05 - 1	02-10-E	9	-0.0379	-	7470A	PPB	12 Feb 2020 11:21:01	U	SMPL
L1456-01LX5 - 1		1612	0.3643	-	7470A	PPB	12 Feb 2020 11:23:08	U	SMPL
L1456-01A - 1		22898	5.7052	-	7470A	PPB	12 Feb 2020 11:25:15	U	SMPL
L1367-04LX5 - 1		63	-0.0244	-	7470A	PPB	12 Feb 2020 11:27:23	U	SMPL
L1367-04A - 1		13640	3.3822	-	7470A	PPB	12 Feb 2020 11:29:30	U	SMPL
PB126754TB - 1	PB126729TB	0	-0.0402	-	7470A	PPB	12 Feb 2020 11:31:36	U	SMPL
CCV15 - 1	CCV15	21216	5.2831	-	7470A	PPB	12 Feb 2020 11:33:42	U	SMPL
CCB15 - 1	CCB15	52	-0.0272	-	7470A	PPB	12 Feb 2020 11:35:49	U	SMPL