


LB107744

245.1

INSTRUMENT ID: CV1

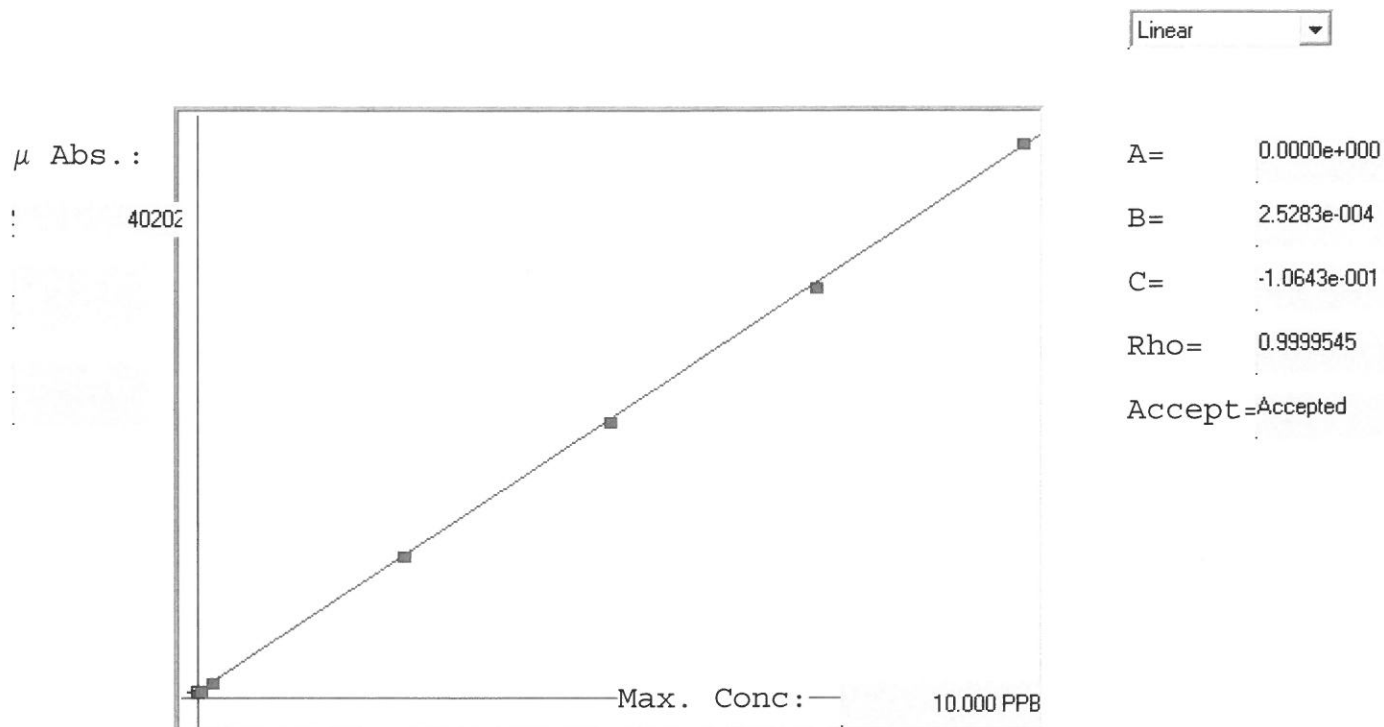

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.019	0.019	497	0.000	497				
0.05	0.050	0.049	-0.001	615	0.0 %	615				
0.2	0.200	0.204	0.004	1227	0.0 %	1227				
2.5	2.500	2.514	0.014	10366	0.0 %	10366				
5.0	5.000	4.967	-0.033	20065	0.0 %	20065				
7.5	7.500	7.439	-0.061	29844	0.0 %	29844				
10.0	10.000	10.058	0.058	40202	0.0 %	40202				

LB107744 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 13 Feb 2020 13:43:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0	497	-	0.0000	245.1	PPB	13 Feb 2020 13:46:22	S	Std
0.05 - 1	S0.05	615	-	0.0500	245.1	PPB	13 Feb 2020 13:48:39	S	Std
0.2 - 1	S0.2	1227	-	0.2000	245.1	PPB	13 Feb 2020 13:50:56	S	Std
2.5 - 1	S2.5	10366	-	2.5000	245.1	PPB	13 Feb 2020 13:53:12	S	Std
5.0 - 1	S5	20065	-	5.0000	245.1	PPB	13 Feb 2020 13:55:28	S	Std
7.5 - 1	S7.5	29844	-	7.5000	245.1	PPB	13 Feb 2020 13:57:44	S	Std
10.0 - 1	S10	40202	-	10.0000	245.1	PPB	13 Feb 2020 14:06:23	S	Std
ICV16 - 1	ICV16	15794	3.8868	-245.1		PPB	13 Feb 2020 14:11:44	U	SMPL
ICB16 - 1	ICB16	596	0.0443	-245.1		PPB	13 Feb 2020 14:13:59	U	SMPL
CCV26 - 1	CCV26	20461	5.0667	-245.1		PPB	13 Feb 2020 14:16:13	U	SMPL
CCB26 - 1	CCB26	494	0.0185	-245.1		PPB	13 Feb 2020 14:21:14	U	SMPL
CRA - 1	CRA	612	0.0483	-245.1		PPB	13 Feb 2020 14:23:28	U	SMPL
HighStd - 1	HighStd	41017	10.2639	-245.1		PPB	13 Feb 2020 14:25:43	U	SMPL
ChkStd - 1	ChkStd	29254	7.2899	-245.1		PPB	13 Feb 2020 14:27:58	U	SMPL
PB126801BL - 1	PBW	433	0.0030	-245.1		PPB	13 Feb 2020 14:35:27	U	SMPL
PB126801BS - 1	LCSW	16958	4.1811	-245.1		PPB	13 Feb 2020 14:37:42	U	SMPL
L1446-01 - 1	HP-640	700	0.0705	-245.1		PPB	13 Feb 2020 14:39:58	U	SMPL
L1446-01DUP - 1	HP-640DUP	717	0.0748	-245.1		PPB	13 Feb 2020 14:42:14	U	SMPL
L1446-01MS - 1	HP-640MS	16731	4.1237	-245.1		PPB	13 Feb 2020 14:44:31	U	SMPL
L1446-01MSD - 1	HP-640MSD	16142	3.9748	-245.1		PPB	13 Feb 2020 14:46:48	U	SMPL
CCV27 - 1	CCV27	20608	5.1039	-245.1		PPB	13 Feb 2020 14:49:03	U	SMPL
CCB27 - 1	CCB27	500	0.0200	-245.1		PPB	13 Feb 2020 14:51:18	U	SMPL
L1446-01LX5 - 1		409	-0.0030	-245.1		PPB	13 Feb 2020 14:53:32	U	SMPL
L1446-01A - 1		16615	4.0943	-245.1		PPB	13 Feb 2020 14:55:48	U	SMPL
CCV28 - 1	CCV28	20512	5.0796	-245.1		PPB	13 Feb 2020 14:58:03	U	SMPL
CCB28 - 1	CCB28	463	0.0106	-245.1		PPB	13 Feb 2020 15:00:18	U	SMPL