


LB 107748

7470A

INSTRUMENT ID : CV1

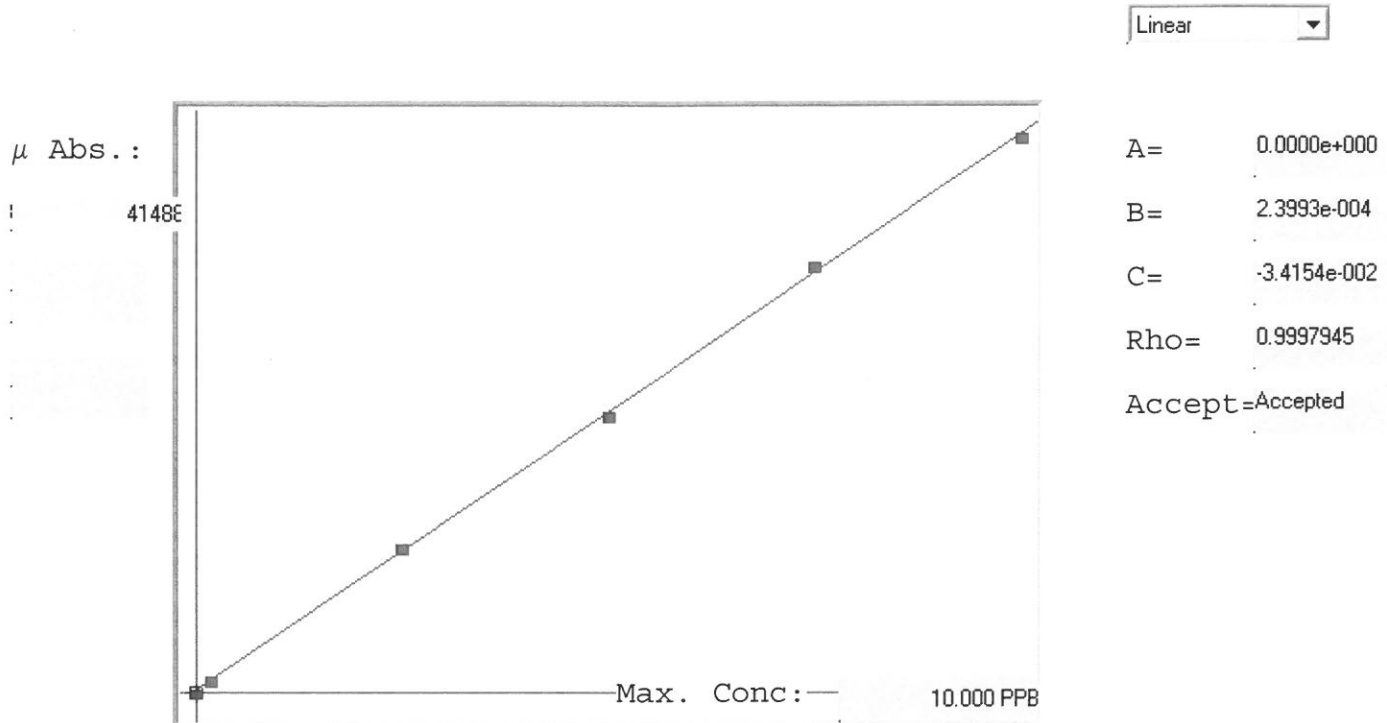

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.023	-0.023	45	0.000	45				
0.2	0.200	0.181	-0.019	895	0.0 %	895				
2.5	2.500	2.566	0.066	10839	0.0 %	10839				
5.0	5.000	4.927	-0.073	20679	0.0 %	20679				
7.5	7.500	7.629	0.129	31938	0.0 %	31938				
10.0	10.000	9.920	-0.080	41488	0.0 %	41488				

LB107748 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 13 Feb 2020 15:12:42					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	45	-	0.0000	7470A	PPB	13 Feb 2020 15:13:44	S	Std
0.2 - 1	50.2	895	-	0.2000	7470A	PPB	13 Feb 2020 15:15:52	S	Std
2.5 - 1	52.5	10839	-	2.5000	7470A	PPB	13 Feb 2020 15:17:59	S	Std
5.0 - 1	55	20679	-	5.0000	7470A	PPB	13 Feb 2020 15:20:07	S	Std
7.5 - 1	57.5	31938	-	7.5000	7470A	PPB	13 Feb 2020 15:22:14	S	Std
10.0 - 1	510	41488	-	10.0000	7470A	PPB	13 Feb 2020 15:24:20	S	Std
ICV17 - 1	ICV17	16442	3.9108	-	7470A	PPB	13 Feb 2020 15:26:52	U	SMPL
ICB17 - 1	ICB17	26	-0.0279	-	7470A	PPB	13 Feb 2020 15:28:58	U	SMPL
CCV29 - 1	CCV29	20434	4.8686	-	7470A	PPB	13 Feb 2020 15:31:03	U	SMPL
CCB29 - 1	CCB29	29	-0.0272	-	7470A	PPB	13 Feb 2020 15:33:09	U	SMPL
CRA - 1	CRA	899	0.1815	-	7470A	PPB	13 Feb 2020 15:35:14	U	SMPL
HighStd - 1	HighStd	41702	9.9715	-	7470A	PPB	13 Feb 2020 15:37:20	U	SMPL
ChkStd - 1	ChkStd	28595	6.8267	-	7470A	PPB	13 Feb 2020 15:39:26	U	SMPL
PB126800BL - 1	PBW	-16	-0.0380	-	7470A	PPB	13 Feb 2020 15:41:32	U	SMPL
PB126800BS - 1	LCSW	16858	4.0106	-	7470A	PPB	13 Feb 2020 15:43:39	U	SMPL
L1370-05 - 1	OR-02-021220	3	-0.0334	-	7470A	PPB	13 Feb 2020 15:45:46	U	SMPL
L1370-05DUP - 1	OR-02-021220DUP	29	-0.0272	-	7470A	PPB	13 Feb 2020 15:47:53	U	SMPL
L1370-05MS - 1	OR-02-021220MS	15659	3.7229	-	7470A	PPB	13 Feb 2020 15:50:01	U	SMPL
L1370-05MSD - 1	OR-02-021220MSD	16818	4.0010	-	7470A	PPB	13 Feb 2020 15:52:09	U	SMPL
L1385-04 - 1	HD-02-021220	4	-0.0332	-	7470A	PPB	13 Feb 2020 15:54:15	U	SMPL
CCV30 - 1	CCV30	20638	4.9176	-	7470A	PPB	13 Feb 2020 15:56:21	U	SMPL
CCB30 - 1	CCB30	29	-0.0272	-	7470A	PPB	13 Feb 2020 15:58:27	U	SMPL
L1505-02 - 1	TEST-PIT-1	23	-0.0286	-	7470A	PPB	13 Feb 2020 16:00:32	U	SMPL
L1509-11 - 1	AOC-3-SP-C	29	-0.0272	-	7470A	PPB	13 Feb 2020 16:02:38	U	SMPL
L1509-12 - 1	AOC-3-SP-D	29	-0.0272	-	7470A	PPB	13 Feb 2020 16:04:45	U	SMPL
L1510-02 - 1	TP-1	21	-0.0291	-	7470A	PPB	13 Feb 2020 16:06:51	U	SMPL
L1510-04 - 1	TP-2	78	-0.0154	-	7470A	PPB	13 Feb 2020 16:08:58	U	SMPL
L1511-02 - 1	LAYDOWN-SOFT-AREA	37	-0.0253	-	7470A	PPB	13 Feb 2020 16:11:05	U	SMPL
L1370-05LX5 - 1		41	-0.0243	-	7470A	PPB	13 Feb 2020 16:13:11	U	SMPL
L1370-05A - 1		17105	4.0699	-	7470A	PPB	13 Feb 2020 16:15:19	U	SMPL
PB126800TB - 1	PB126780TB	26	-0.0279	-	7470A	PPB	13 Feb 2020 16:17:26	U	SMPL
CCV31 - 1	CCV31	20572	4.9017	-	7470A	PPB	13 Feb 2020 16:19:32	U	SMPL
CCB31 - 1	CCB31	45	-0.0234	-	7470A	PPB	13 Feb 2020 16:21:38	U	SMPL