


LB107804

7470A

INSTRUMENT ID: CV1

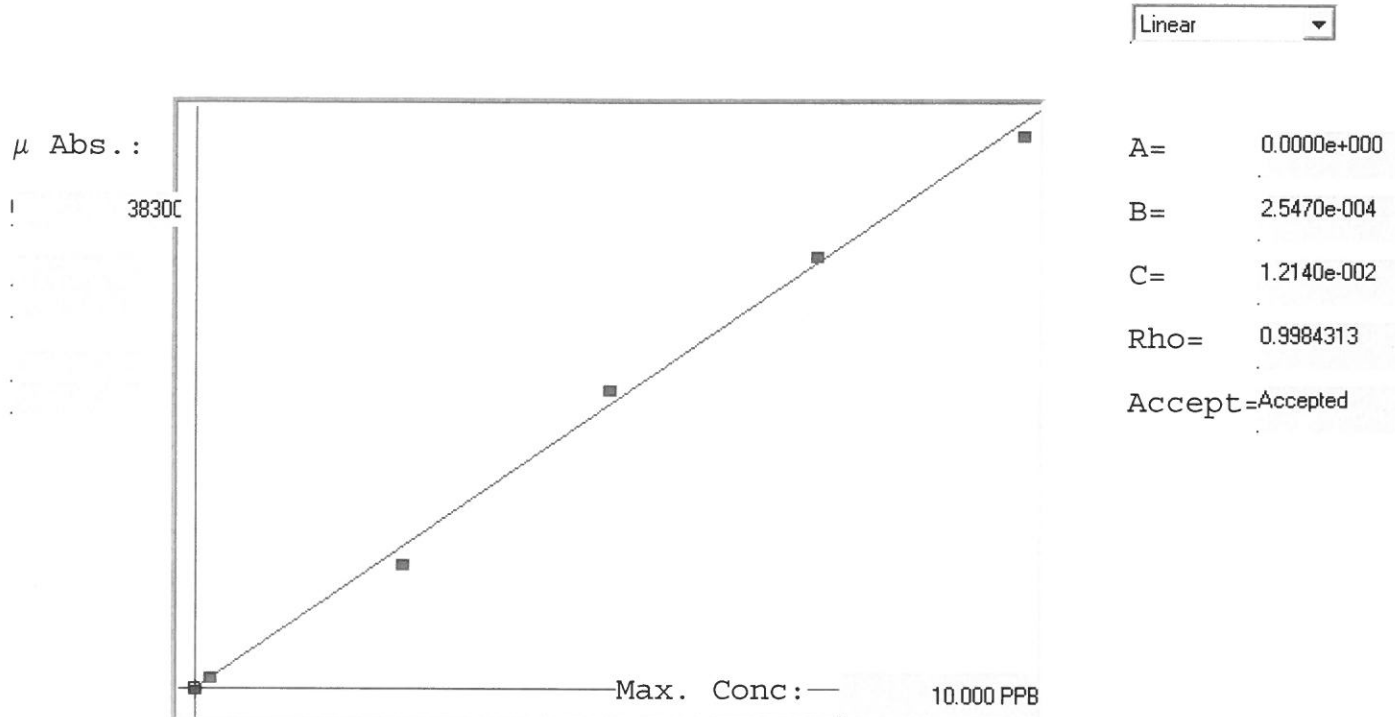

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	8	0.000	8				
0.2	0.200	0.233	0.033	867	0.0 %	867				
2.5	2.500	2.215	-0.285	8649	0.0 %	8649				
5.0	5.000	5.301	0.301	20764	0.0 %	20764				
7.5	7.500	7.670	0.170	30067	0.0 %	30067				
10.0	10.000	9.767	-0.233	38300	0.0 %	38300				

LB107804 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Feb 2020 09:22:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	8	-	0.0000	7470A	PPB	18 Feb 2020 09:25:08	S	Std
0.2 - 1	50.2	867	-	0.2000	7470A	PPB	18 Feb 2020 09:27:15	S	Std
2.5 - 1	52.5	8649	-	2.5000	7470A	PPB	18 Feb 2020 09:29:23	S	Std
5.0 - 1	55	20764	-	5.0000	7470A	PPB	18 Feb 2020 09:31:31	S	Std
7.5 - 1	57.5	30067	-	7.5000	7470A	PPB	18 Feb 2020 09:33:38	S	Std
10.0 - 1	510	38300	-	10.0000	7470A	PPB	18 Feb 2020 09:40:31	S	Std
ICV20 - 1	ICV20	15893	4.0600	-	7470A	PPB	18 Feb 2020 09:43:13	U	SMPL
ICB20 - 1	ICB20	-23	0.0063	-	7470A	PPB	18 Feb 2020 09:45:18	U	SMPL
CCV43 - 1	CCV43	20104	5.1326	-	7470A	PPB	18 Feb 2020 09:47:23	U	SMPL
CCB43 - 1	CCB43	-36	0.0030	-	7470A	PPB	18 Feb 2020 09:49:29	U	SMPL
CRA - 1	CRA	862	0.2317	-	7470A	PPB	18 Feb 2020 09:51:34	U	SMPL
HighStd - 1	HighStd	38089	9.7133	-	7470A	PPB	18 Feb 2020 09:53:40	U	SMPL
ChkStd - 1	ChkStd	29359	7.4898	-	7470A	PPB	18 Feb 2020 09:55:46	U	SMPL
PB126871BL - 1	PBW	-48	-0.0001	-	7470A	PPB	18 Feb 2020 09:57:52	U	SMPL
PB126871BS - 1	LCSW	16487	4.2113	-	7470A	PPB	18 Feb 2020 09:59:59	U	SMPL
L1365-16 - 1	CL-02-021420	-6	0.0106	-	7470A	PPB	18 Feb 2020 10:02:06	U	SMPL
L1365-16DUP - 1	CL-02-021420DUP	4	0.0132	-	7470A	PPB	18 Feb 2020 10:04:12	U	SMPL
L1365-16MS - 1	CL-02-021420MS	15190	3.8810	-	7470A	PPB	18 Feb 2020 10:06:19	U	SMPL
L1365-16MSD - 1	CL-02-021420MSD	16562	4.2304	-	7470A	PPB	18 Feb 2020 10:08:27	U	SMPL
L1530-01 - 1	IDW-MCM-200213	0	0.0121	-	7470A	PPB	18 Feb 2020 10:10:33	U	SMPL
CCV44 - 1	CCV44	20271	5.1751	-	7470A	PPB	18 Feb 2020 10:12:38	U	SMPL
CCB44 - 1	CCB44	-18	0.0076	-	7470A	PPB	18 Feb 2020 10:14:44	U	SMPL
L1530-02 - 1	IDW-LGAC-200213	8	0.0142	-	7470A	PPB	18 Feb 2020 10:16:50	U	SMPL
L1530-03 - 1	IDW-GS-200213	-7	0.0104	-	7470A	PPB	18 Feb 2020 10:18:55	U	SMPL
L1530-04 - 1	IDW-VCAG-200213	-3	0.0114	-	7470A	PPB	18 Feb 2020 10:21:01	U	SMPL
L1544-03 - 1	2-5-1	0	0.0121	-	7470A	PPB	18 Feb 2020 10:23:08	U	SMPL
L1544-07 - 1	2-4-1	0	0.0121	-	7470A	PPB	18 Feb 2020 10:25:14	U	SMPL
L1365-16LX5 - 1		-17	0.0078	-	7470A	PPB	18 Feb 2020 10:27:21	U	SMPL
L1365-16A - 1		15823	4.0422	-	7470A	PPB	18 Feb 2020 10:29:29	U	SMPL
PB126871TB - 1	PB126833TB	-22	0.0065	-	7470A	PPB	18 Feb 2020 10:31:36	U	SMPL
CCV45 - 1	CCV45	20256	5.1713	-	7470A	PPB	18 Feb 2020 10:33:44	U	SMPL
CCB45 - 1	CCB45	-20	0.0070	-	7470A	PPB	18 Feb 2020 10:35:50	U	SMPL