


LB107806

7471B

INSTRUMENT ID: CX1

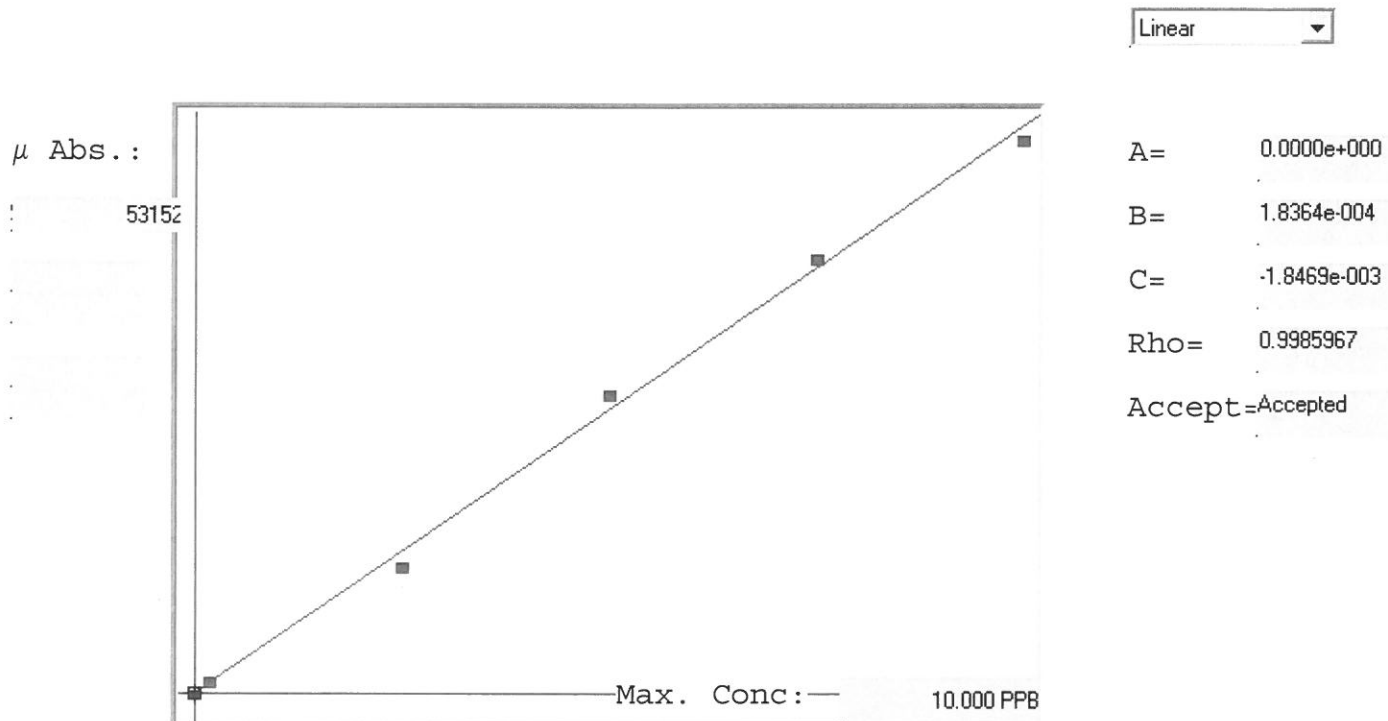

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.004	0.004	30	0.000	30				
0.2	0.200	0.216	0.016	1188	0.0 %	1188				
2.5	2.500	2.257	-0.243	12302	0.0 %	12302				
5.0	5.000	5.277	0.277	28748	0.0 %	28748				
7.5	7.500	7.687	0.187	41868	0.0 %	41868				
10.0	10.000	9.759	-0.241	53152	0.0 %	53152				

LB107806 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 18 Feb 2020 11:17:21					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	30	-	0.0000	7471B	PPB	18 Feb 2020 11:20:30	S	Std
0.2 - 1	SD 2	1188	-	0.2000	7471B	PPB	18 Feb 2020 11:22:47	S	Std
2.5 - 1	SD 5	12302	-	2.5000	7471B	PPB	18 Feb 2020 11:25:04	S	Std
5.0 - 1	SD	28748	-	5.0000	7471B	PPB	18 Feb 2020 11:27:21	S	Std
7.5 - 1	SD 5	41868	-	7.5000	7471B	PPB	18 Feb 2020 11:29:37	S	Std
10.0 - 1	SD	53152	-	10.0000	7471B	PPB	18 Feb 2020 11:31:53	S	Std
ICV21 - 1	ICV21	23326	4.2817	-	7471B	PPB	18 Feb 2020 11:34:43	U	SMPL
ICB21 - 1	ICB21	-19	-0.0053	-	7471B	PPB	18 Feb 2020 11:36:57	U	SMPL
CCV46 - 1	CCV46	29080	5.3383	-	7471B	PPB	18 Feb 2020 11:39:12	U	SMPL
CCB46 - 1	CCB46	-33	-0.0079	-	7471B	PPB	18 Feb 2020 11:41:27	U	SMPL
CRA - 1	CRA	1176	0.2141	-	7471B	PPB	18 Feb 2020 11:43:42	U	SMPL
HighStd - 1	HighStd	53113	9.7516	-	7471B	PPB	18 Feb 2020 11:45:56	U	SMPL
ChkStd - 1	ChkStd	42022	7.7149	-	7471B	PPB	18 Feb 2020 11:48:11	U	SMPL
PB126876BL - 1	PBS	-42	-0.0096	-	7471B	PPB	18 Feb 2020 11:50:28	U	SMPL
PB126876BS - 1	LCSS	22858	4.1957	-	7471B	PPB	18 Feb 2020 11:52:43	U	SMPL
L1551-01 - 1	FK-SF-01-007-A	9289	1.7040	-	7471B	PPB	18 Feb 2020 11:54:59	U	SMPL
L1551-01DUP - 1	FK-SF-01-007-ADUP	9288	1.7038	-	7471B	PPB	18 Feb 2020 11:57:15	U	SMPL
L1551-01MS - 1	FK-SF-01-007-AMS	31428	5.7695	-	7471B	PPB	18 Feb 2020 11:59:32	U	SMPL
L1551-01MSD - 1	FK-SF-01-007-AMSD	30801	5.6543	-	7471B	PPB	18 Feb 2020 12:01:49	U	SMPL
L1551-03 - 1	FK-SF-01-007-B	7269	1.3330	-	7471B	PPB	18 Feb 2020 12:04:04	U	SMPL
CCV47 - 1	CCV47	28441	5.2210	-	7471B	PPB	18 Feb 2020 12:06:19	U	SMPL
CCB47 - 1	CCB47	-16	-0.0048	-	7471B	PPB	18 Feb 2020 12:08:34	U	SMPL
L1552-01 - 1	FK-SF-01-008-A	7393	1.3558	-	7471B	PPB	18 Feb 2020 12:10:50	U	SMPL
L1552-03 - 1	FK-SF-01-008-B	6896	1.2645	-	7471B	PPB	18 Feb 2020 12:13:05	U	SMPL
L1558-01 - 1	0166-COMP-BT-A	3467	0.6348	-	7471B	PPB	18 Feb 2020 12:15:21	U	SMPL
L1558-02 - 1	0167-COMP-BT-B	3759	0.6884	-	7471B	PPB	18 Feb 2020 12:17:36	U	SMPL
L1558-03 - 1	0168-COMP-CM-A	5495	1.0072	-	7471B	PPB	18 Feb 2020 12:19:51	U	SMPL
L1558-04 - 1	0169-COMP-BC-A	5190	0.9512	-	7471B	PPB	18 Feb 2020 12:22:08	U	SMPL
L1551-01LX5 - 1		1854	0.3386	-	7471B	PPB	18 Feb 2020 12:24:24	U	SMPL
L1551-01A - 1		30191	5.5423	-	7471B	PPB	18 Feb 2020 12:26:41	U	SMPL
CCV48 - 1	CCV48	29173	5.3554	-	7471B	PPB	18 Feb 2020 12:28:58	U	SMPL
CCB48 - 1	CCB48	4	-0.0011	-	7471B	PPB	18 Feb 2020 12:31:14	U	SMPL