


LB107831

INSTRUMENT ID: CV1

245.1

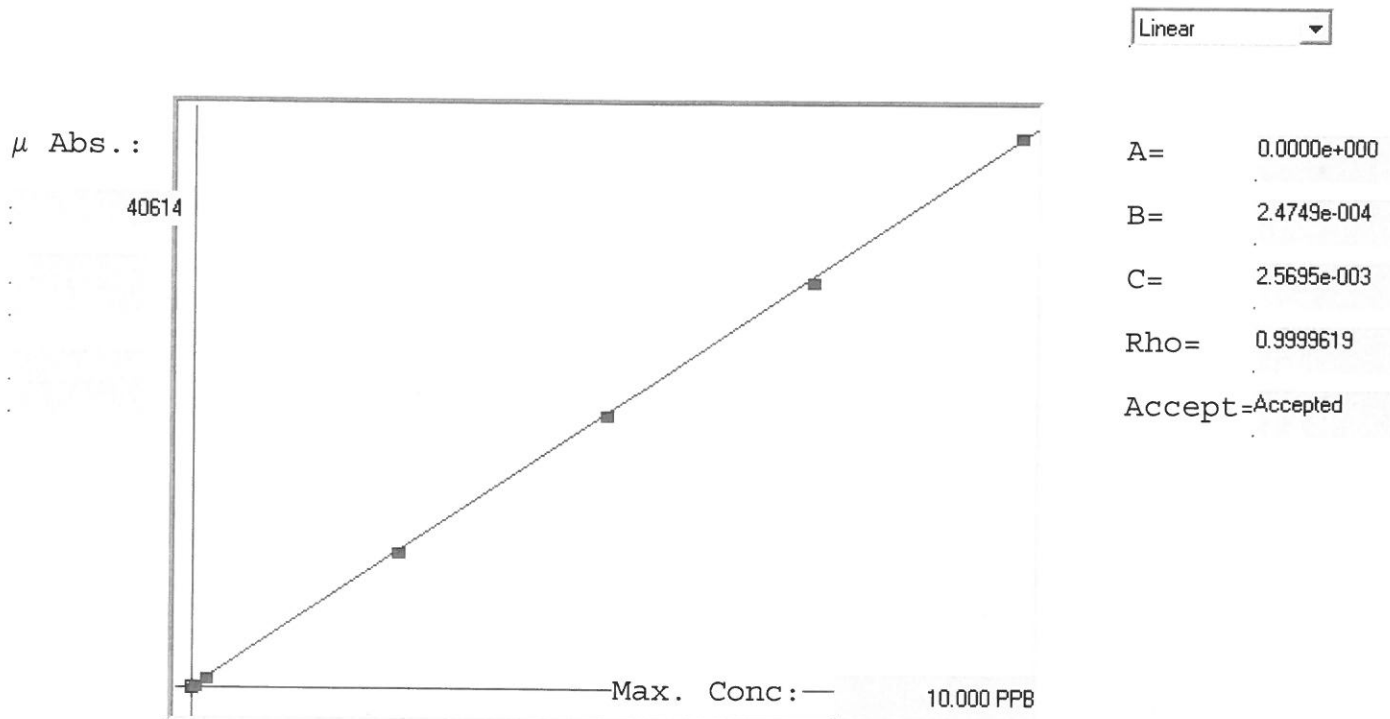

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.010	0.010	32	0.000	32				
0.05	0.050	0.055	0.005	212	0.0 %	212				
0.2	0.200	0.211	0.011	842	0.0 %	842				
2.5	2.500	2.497	-0.003	10079	0.0 %	10079				
5.0	5.000	4.985	-0.015	20130	0.0 %	20130				
7.5	7.500	7.438	-0.062	30041	0.0 %	30041				
10.0	10.000	10.054	0.054	40614	0.0 %	40614				

LB107831 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 19 Feb 2020 11:42:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	32	-	0.0000	245.1	PPB	19 Feb 2020 11:46:09	S	Std
0.05 - 1	50.05	212	-	0.0500	245.1	PPB	19 Feb 2020 11:48:26	S	Std
0.2 - 1	50.2	842	-	0.2000	245.1	PPB	19 Feb 2020 11:50:43	S	Std
2.5 - 1	52.5	10079	-	2.5000	245.1	PPB	19 Feb 2020 11:53:00	S	Std
5.0 - 1	55	20130	-	5.0000	245.1	PPB	19 Feb 2020 11:55:16	S	Std
7.5 - 1	57.5	30041	-	7.5000	245.1	PPB	19 Feb 2020 11:57:32	S	Std
10.0 - 1	510	40614	-	10.0000	245.1	PPB	19 Feb 2020 11:59:47	S	Std
ICV23 - 1	ICV23	15388	3.8110	-245.1		PPB	19 Feb 2020 12:05:01	U	SMPL
ICB23 - 1	ICB23	-13	-0.0006	-245.1		PPB	19 Feb 2020 12:07:15	U	SMPL
CCV52 - 1	CCV52	20462	5.0668	-245.1		PPB	19 Feb 2020 12:09:30	U	SMPL
CCB52 - 1	CCB52	-20	-0.0024	-245.1		PPB	19 Feb 2020 12:11:45	U	SMPL
CRA - 1	CRA	208	0.0540	-245.1		PPB	19 Feb 2020 12:14:00	U	SMPL
HighStd - 1	HighStd	41733	10.3312	-245.1		PPB	19 Feb 2020 12:16:14	U	SMPL
ChkStd - 1	ChkStd	29042	7.1903	-245.1		PPB	19 Feb 2020 12:18:30	U	SMPL
PB126920BL - 1	PBW	-41	-0.0076	-245.1		PPB	19 Feb 2020 12:20:45	U	SMPL
PB126920BS - 1	LCSW	15749	3.9004	-245.1		PPB	19 Feb 2020 12:23:01	U	SMPL
L1561-01 - 1	MANHOLE	7	0.0043	-245.1		PPB	19 Feb 2020 12:25:18	U	SMPL
L1561-01DUP - 1	MANHOLEDUP	39	0.0122	-245.1		PPB	19 Feb 2020 12:27:34	U	SMPL
L1561-01MS - 1	MANHOLEMS	15623	3.8692	-245.1		PPB	19 Feb 2020 12:29:51	U	SMPL
L1561-01MSD - 1	MANHOLEMSD	16293	4.0350	-245.1		PPB	19 Feb 2020 12:32:08	U	SMPL
CCV53 - 1	CCV53	19398	4.8035	-245.1		PPB	19 Feb 2020 12:34:23	U	SMPL
CCB53 - 1	CCB53	-19	-0.0021	-245.1		PPB	19 Feb 2020 12:36:38	U	SMPL
L1561-01LX5 - 1		10	0.0050	-245.1		PPB	19 Feb 2020 12:38:54	U	SMPL
L1561-01A - 1		15613	3.8667	-245.1		PPB	19 Feb 2020 12:41:09	U	SMPL
CCV54 - 1	CCV54	19383	4.7997	-245.1		PPB	19 Feb 2020 12:43:25	U	SMPL
CCB54 - 1	CCB54	-12	-0.0004	-245.1		PPB	19 Feb 2020 12:45:40	U	SMPL