


LB107840

7470A

INSTRUMENT ID : CV1

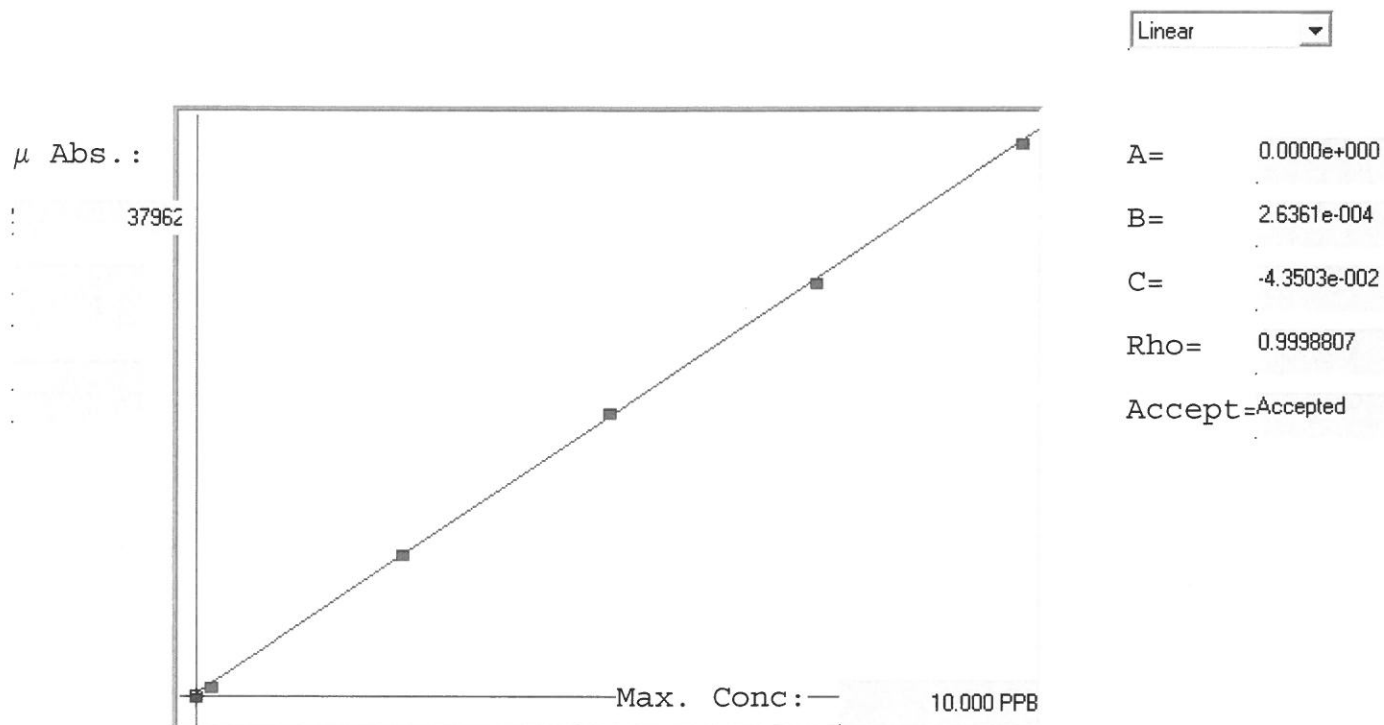

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.032	-0.032	44	0.000	44				
0.2	0.200	0.158	-0.042	763	0.0 %	763				
2.5	2.500	2.540	0.040	9802	0.0 %	9802				
5.0	5.000	5.110	0.110	19550	0.0 %	19550				
7.5	7.500	7.460	-0.040	28464	0.0 %	28464				
10.0	10.000	9.964	-0.036	37962	0.0 %	37962				

LB107840 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 19 Feb 2020 13:49:21

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	44	-	0.0000	7470A	PPB	19 Feb 2020 13:50:38	S	Std
0.2 - 1	50.2	763	-	0.2000	7470A	PPB	19 Feb 2020 13:52:46	S	Std
2.5 - 1	52.5	9802	-	2.5000	7470A	PPB	19 Feb 2020 13:54:53	S	Std
5.0 - 1	55	19550	-	5.0000	7470A	PPB	19 Feb 2020 13:57:00	S	Std
7.5 - 1	57.5	28464	-	7.5000	7470A	PPB	19 Feb 2020 13:59:07	S	Std
10.0 - 1	50	37962	-	10.0000	7470A	PPB	19 Feb 2020 14:01:13	S	Std
ICV24 - 1	ICV24	14432	3.7610	-	7470A	PPB	19 Feb 2020 14:03:58	U	SMPL
ICB24 - 1	ICB24	0	-0.0435	-	7470A	PPB	19 Feb 2020 14:06:03	U	SMPL
CCV55 - 1	CCV55	20120	5.2604	-	7470A	PPB	19 Feb 2020 14:08:09	U	SMPL
CCB55 - 1	CCB55	0	-0.0435	-	7470A	PPB	19 Feb 2020 14:10:15	U	SMPL
CRA - 1	CRA	756	0.1558	-	7470A	PPB	19 Feb 2020 14:12:20	U	SMPL
HighStd - 1	HighStd	38787	10.1812	-	7470A	PPB	19 Feb 2020 14:14:26	U	SMPL
ChkStd - 1	ChkStd	26963	7.0643	-	7470A	PPB	19 Feb 2020 14:16:31	U	SMPL
PB126921BL - 1	PBW	-12	-0.0467	-	7470A	PPB	19 Feb 2020 14:18:38	U	SMPL
PB126921BS - 1	LCSW	16179	4.2215	-	7470A	PPB	19 Feb 2020 14:20:44	U	SMPL
L1362-03 - 1	BU-03-021820	0	-0.0435	-	7470A	PPB	19 Feb 2020 14:22:51	U	SMPL
L1362-03DUP - 1	BU-03-021820DUP	31	-0.0353	-	7470A	PPB	19 Feb 2020 14:24:59	U	SMPL
L1362-03MS - 1	BU-03-021820MS	13749	3.5809	-	7470A	PPB	19 Feb 2020 14:27:06	U	SMPL
L1362-03MSD - 1	BU-03-021820MSD	14033	3.6558	-	7470A	PPB	19 Feb 2020 14:29:14	U	SMPL
L1567-01 - 1	02-18-A	14	-0.0398	-	7470A	PPB	19 Feb 2020 14:31:20	U	SMPL
CCV56 - 1	CCV56	19969	5.2206	-	7470A	PPB	19 Feb 2020 14:33:26	U	SMPL
CCB56 - 1	CCB56	-8	-0.0456	-	7470A	PPB	19 Feb 2020 14:35:33	U	SMPL
L1567-02 - 1	02-18-B	35	-0.0343	-	7470A	PPB	19 Feb 2020 14:37:39	U	SMPL
L1567-03 - 1	02-18-C	24	-0.0372	-	7470A	PPB	19 Feb 2020 14:39:44	U	SMPL
L1567-04 - 1	02-18-D	38	-0.0335	-	7470A	PPB	19 Feb 2020 14:41:50	U	SMPL
L1567-05 - 1	02-18-E	35	-0.0343	-	7470A	PPB	19 Feb 2020 14:43:56	U	SMPL
L1567-06 - 1	02-18-F	44	-0.0319	-	7470A	PPB	19 Feb 2020 14:46:02	U	SMPL
L1573-01 - 1	LOC-1	34	-0.0345	-	7470A	PPB	19 Feb 2020 14:48:09	U	SMPL
L1573-03 - 1	LOC-2	38	-0.0335	-	7470A	PPB	19 Feb 2020 14:50:16	U	SMPL
L1573-05 - 1	LOC-3	28	-0.0361	-	7470A	PPB	19 Feb 2020 14:52:23	U	SMPL
L1575-04 - 1	TP-A-S	24	-0.0372	-	7470A	PPB	19 Feb 2020 14:54:31	U	SMPL
L1575-08 - 1	TP-A-D	26	-0.0366	-	7470A	PPB	19 Feb 2020 14:56:37	U	SMPL
CCV57 - 1	CCV57	20024	5.2351	-	7470A	PPB	19 Feb 2020 14:58:43	U	SMPL
CCB57 - 1	CCB57	-2	-0.0440	-	7470A	PPB	19 Feb 2020 15:00:50	U	SMPL
PB126922BL - 1	PBW	20	-0.0382	-	7470A	PPB	19 Feb 2020 15:02:56	U	SMPL
PB126922BS - 1	LCSW	15453	4.0301	-	7470A	PPB	19 Feb 2020 15:05:02	U	SMPL
L1577-01 - 1	WFD-GW-01-23	316	0.0398	-	7470A	PPB	19 Feb 2020 15:07:08	U	SMPL
L1577-01DUP - 1	WFD-GW-01-23DUP	172	0.0018	-	7470A	PPB	19 Feb 2020 15:09:14	U	SMPL
L1577-01MS - 1	WFD-GW-01-23MS	15081	3.9320	-	7470A	PPB	19 Feb 2020 15:11:20	U	SMPL
L1577-01MSD - 1	WFD-GW-01-23MSD	15796	4.1205	-	7470A	PPB	19 Feb 2020 15:13:27	U	SMPL
L1578-02 - 1	WFD-WC-L-01	17	-0.0390	-	7470A	PPB	19 Feb 2020 15:15:34	U	SMPL
CCV58 - 1	CCV58	19583	5.1188	-	7470A	PPB	19 Feb 2020 15:17:41	U	SMPL
CCB58 - 1	CCB58	10	-0.0409	-	7470A	PPB	19 Feb 2020 15:19:49	U	SMPL
L1362-03LX5 - 1		25	-0.0369	-	7470A	PPB	19 Feb 2020 15:21:55	U	SMPL
L1362-03A - 1		14709	3.8340	-	7470A	PPB	19 Feb 2020 15:24:01	U	SMPL
L1577-01LX5 - 1		57	-0.0285	-	7470A	PPB	19 Feb 2020 15:26:08	U	SMPL
L1577-01A - 1		16238	4.2370	-	7470A	PPB	19 Feb 2020 15:28:13	U	SMPL
PB126921TB - 1	PB126909TB	34	-0.0345	-	7470A	PPB	19 Feb 2020 15:35:32	U	SMPL
CCV59 - 1	CCV59	19718	5.1544	-	7470A	PPB	19 Feb 2020 15:37:38	U	SMPL
CCB59 - 1	CCB59	-5	-0.0448	-	7470A	PPB	19 Feb 2020 15:39:44	U	SMPL