


LB107871

7470A

INSTRUMENT ID: CV1

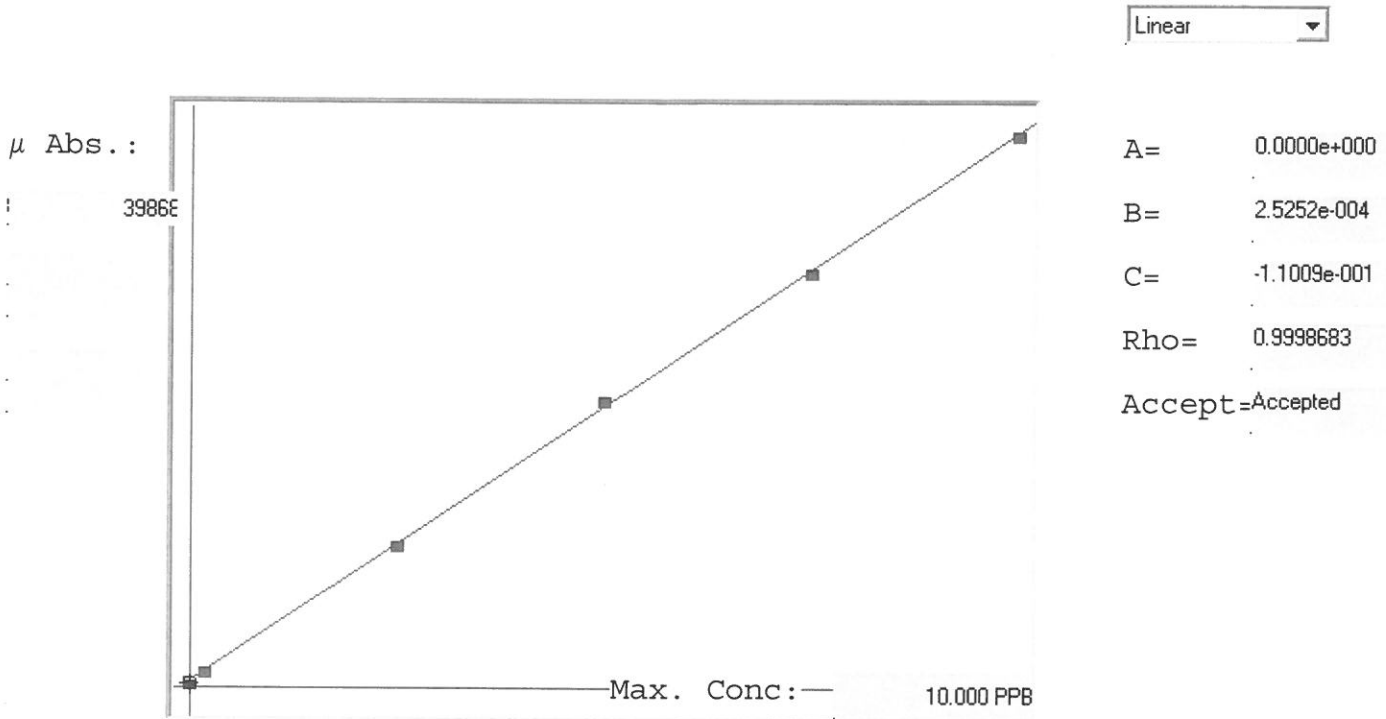

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	347	0.000	347				
0.2	0.200	0.172	-0.028	1119	0.0 %	1119				
2.5	2.500	2.491	-0.009	10300	0.0 %	10300				
5.0	5.000	5.132	0.132	20759	0.0 %	20759				
7.5	7.500	7.469	-0.031	30015	0.0 %	30015				
10.0	10.000	9.958	-0.042	39868	0.0 %	39868				

LB107871 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Feb 2020 14:59:50

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	347	-	0.0007470A	PPB		20 Feb 2020 15:01:08	S	Std
0.2 - 1	50.2	1119	-	0.20007470A	PPB		20 Feb 2020 15:03:16	S	Std
2.5 - 1	52.5	10300	-	2.50007470A	PPB		20 Feb 2020 15:05:23	S	Std
5.0 - 1	55	20759	-	5.00007470A	PPB		20 Feb 2020 15:07:31	S	Std
7.5 - 1	57.5	30015	-	7.50007470A	PPB		20 Feb 2020 15:09:37	S	Std
10.0 - 1	59	39868	-	10.00007470A	PPB		20 Feb 2020 15:11:43	S	Std
ICV26 - 1	ICV26	15010	3.6803	-7470A	PPB		20 Feb 2020 15:14:14	U	SMPL
ICB26 - 1	ICB26	280	-0.0394	-7470A	PPB		20 Feb 2020 15:16:19	U	SMPL
CCV66 - 1	CCV66	19189	4.7356	-7470A	PPB		20 Feb 2020 15:18:25	U	SMPL
CCB66 - 1	CCB66	288	-0.0374	-7470A	PPB		20 Feb 2020 15:20:30	U	SMPL
CRA - 1	CRA	1126	0.1743	-7470A	PPB		20 Feb 2020 15:22:36	U	SMPL
HighStd - 1	HighStd	40188	10.0384	-7470A	PPB		20 Feb 2020 15:24:41	U	SMPL
ChkStd - 1	ChkStd	27472	6.8273	-7470A	PPB		20 Feb 2020 15:26:47	U	SMPL
PB126957BL - 1	PBW	264	-0.0434	-7470A	PPB		20 Feb 2020 15:28:53	U	SMPL
PB126957BS - 1	LCSW	14305	3.5023	-7470A	PPB		20 Feb 2020 15:31:00	U	SMPL
L1578-01 - 1	WFD-WC-S-SB-010203	295	-0.0356	-7470A	PPB		20 Feb 2020 15:33:07	U	SMPL
L1600-04 - 1	TP-B-S	306	-0.0328	-7470A	PPB		20 Feb 2020 15:35:14	U	SMPL
L1600-08 - 1	TP-B-D	275	-0.0406	-7470A	PPB		20 Feb 2020 15:37:21	U	SMPL
L1600-08DUP - 1	TP-B-DDUP	337	-0.0250	-7470A	PPB		20 Feb 2020 15:39:29	U	SMPL
L1600-08MS - 1	TP-B-DMS	14940	3.6626	-7470A	PPB		20 Feb 2020 15:41:36	U	SMPL
CCV67 - 1	CCV67	20225	4.9972	-7470A	PPB		20 Feb 2020 15:43:42	U	SMPL
CCB67 - 1	CCB67	307	-0.0326	-7470A	PPB		20 Feb 2020 15:45:48	U	SMPL
L1600-08MSD - 1	TP-B-DMSD	13723	3.3553	-7470A	PPB		20 Feb 2020 15:47:54	U	SMPL
PB126958BL - 1	PBW	311	-0.0316	-7470A	PPB		20 Feb 2020 15:50:00	U	SMPL
PB126958BS - 1	LCSW	13998	3.4247	-7470A	PPB		20 Feb 2020 15:52:06	U	SMPL
L1581-01 - 1	40729	383	-0.0134	-7470A	PPB		20 Feb 2020 15:54:12	U	SMPL
L1583-01 - 1	40708	984	0.1384	-7470A	PPB		20 Feb 2020 15:56:19	U	SMPL
L1586-01 - 1	0173-COMP-BT-A-MOD-ELUTRIATE	437	0.0003	-7470A	PPB		20 Feb 2020 15:58:26	U	SMPL
L1586-01DUP - 1	0173-COMP-BT-A-MOD-ELUTRIATEDUP	363	-0.0184	-7470A	PPB		20 Feb 2020 16:00:32	U	SMPL
L1586-01MS - 1	0173-COMP-BT-A-MOD-ELUTRIATEMS	15936	3.9141	-7470A	PPB		20 Feb 2020 16:02:39	U	SMPL
L1586-01MSD - 1	0173-COMP-BT-A-MOD-ELUTRIATEMSD	15691	3.8523	-7470A	PPB		20 Feb 2020 16:04:47	U	SMPL
L1586-02 - 1	0174-COMP-BT-B-MOD-ELUTRIATE	42	-0.0995	-7470A	PPB		20 Feb 2020 16:06:53	U	SMPL
CCV68 - 1	CCV68	20830	5.1500	-7470A	PPB		20 Feb 2020 16:08:59	U	SMPL
CCB68 - 1	CCB68	226	-0.0530	-7470A	PPB		20 Feb 2020 16:11:05	U	SMPL
L1586-03 - 1	0175-COMP-CM-A-MOD-ELUTRIATE	400	-0.0091	-7470A	PPB		20 Feb 2020 16:13:12	U	SMPL
L1586-04 - 1	0176-COMP-BC-A-MOD-ELUTRIATE	415	-0.0053	-7470A	PPB		20 Feb 2020 16:15:18	U	SMPL
L1600-08LX5 - 1		209	-0.0573	-7470A	PPB		20 Feb 2020 16:17:24	U	SMPL
L1600-08A - 1		15034	3.6864	-7470A	PPB		20 Feb 2020 16:19:30	U	SMPL
L1586-01LX5 - 1		269	-0.0422	-7470A	PPB		20 Feb 2020 16:21:37	U	SMPL
L1586-01A - 1		15230	3.7359	-7470A	PPB		20 Feb 2020 16:23:44	U	SMPL
PB126957TB - 1	PB126925TB	308	-0.0323	-7470A	PPB		20 Feb 2020 16:25:51	U	SMPL
CCV69 - 1	CCV69	19658	4.8540	-7470A	PPB		20 Feb 2020 16:27:59	U	SMPL
CCB69 - 1	CCB69	293	-0.0361	-7470A	PPB		20 Feb 2020 16:30:07	U	SMPL