


LB108063

7471B

INSTRUMENT ID: LV1

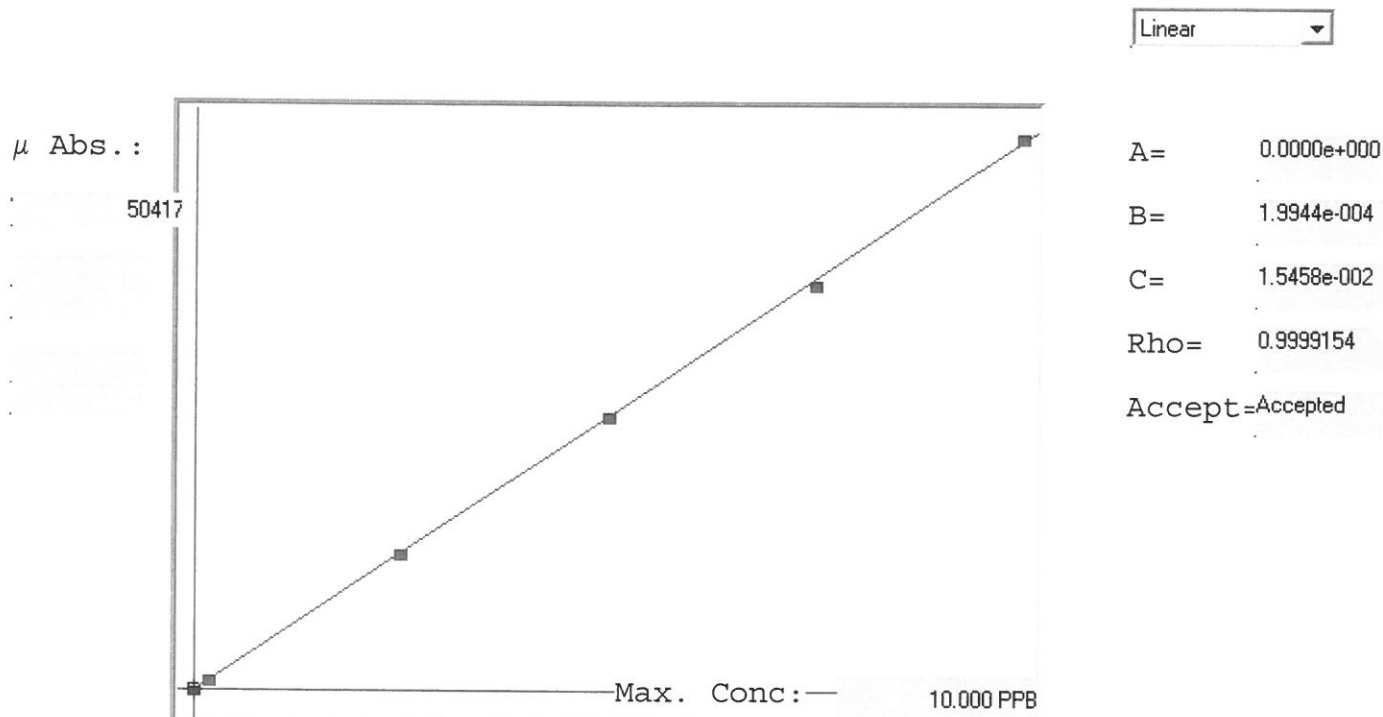

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.016	0.016	4	0.000	4				
0.2	0.200	0.210	0.010	974	0.0 %	974				
2.5	2.500	2.504	0.004	12478	0.0 %	12478				
5.0	5.000	4.991	-0.009	24947	0.0 %	24947				
7.5	7.500	7.408	-0.092	37069	0.0 %	37069				
10.0	10.000	10.071	0.071	50417	0.0 %	50417				

LB108063 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 03 Mar 2020 11:11:27

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	4	-	0.00007471B	PPB	03 Mar 2020 11:20:35	S	Std
0.2 - 1	50.2	974	-	0.20007471B	PPB	03 Mar 2020 11:22:52	S	Std
2.5 - 1	52.5	12478	-	2.50007471B	PPB	03 Mar 2020 11:25:09	S	Std
5.0 - 1	55	24947	-	5.00007471B	PPB	03 Mar 2020 11:27:25	S	Std
7.5 - 1	57.5	37069	-	7.50007471B	PPB	03 Mar 2020 11:29:42	S	Std
10.0 - 1	510	50417	-	10.00007471B	PPB	03 Mar 2020 11:34:43	S	Std
ICV42 - 1	ICV42	20037	4.0116	-7471B	PPB	03 Mar 2020 11:37:27	U	SMPL
ICB42 - 1	ICB42	-364	-0.0571	-7471B	PPB	03 Mar 2020 11:39:44	U	SMPL
CCV43 - 1	CCV43	24864	4.9743	-7471B	PPB	03 Mar 2020 11:42:00	U	SMPL
CCB43 - 1	CCB43	-337	-0.0518	-7471B	PPB	03 Mar 2020 11:44:15	U	SMPL
CRA - 1	CRA	880	0.1910	-7471B	PPB	03 Mar 2020 11:46:31	U	SMPL
HighStd - 1	HighStd	50766	10.1402	-7471B	PPB	03 Mar 2020 11:48:46	U	SMPL
ChkStd - 1	ChkStd	34976	6.9911	-7471B	PPB	03 Mar 2020 11:51:01	U	SMPL
PB127231BL - 1	PBS	-484	-0.0811	-7471B	PPB	03 Mar 2020 11:53:19	U	SMPL
PB127231BS - 1	LCSS	19046	3.8140	-7471B	PPB	03 Mar 2020 11:55:37	U	SMPL
L1683-22 - 1	OF-3-20200225	13896	2.7869	-7471B	PPB	03 Mar 2020 11:57:53	U	SMPL
L1683-23 - 1	OF-2-20200225	335882	67.0036	-7471B	PPB	03 Mar 2020 12:10:08	U	SMPL
L1683-30 - 1	L1683-22MS	31192	6.2364	-7471B	PPB	03 Mar 2020 12:12:25	U	SMPL
L1683-31 - 1	L1683-22MSD	31556	6.3090	-7471B	PPB	03 Mar 2020 12:17:26	U	SMPL
CCV44 - 1	CCV44	26127	5.2262	-7471B	PPB	03 Mar 2020 12:19:40	U	SMPL
CCB44 - 1	CCB44	-99	-0.0043	-7471B	PPB	03 Mar 2020 12:21:57	U	SMPL
L1743-02 - 1	C-7	49577	9.9031	-7471B	PPB	03 Mar 2020 12:24:12	U	SMPL
L1743-04 - 1	C-8	45244	9.0389	-7471B	PPB	03 Mar 2020 12:26:28	U	SMPL
L1743-06 - 1	C-9	3947	0.8026	-7471B	PPB	03 Mar 2020 12:28:44	U	SMPL
L1743-08 - 1	C-3	23746	4.7514	-7471B	PPB	03 Mar 2020 12:31:01	U	SMPL
L1743-10 - 1	C-4	11162	2.2416	-7471B	PPB	03 Mar 2020 12:33:17	U	SMPL
L1743-12 - 1	C-5	2203	0.4548	-7471B	PPB	03 Mar 2020 12:35:33	U	SMPL
L1743-14 - 1	C-6	5605	1.1333	-7471B	PPB	03 Mar 2020 12:37:50	U	SMPL
L1743-16 - 1	C-1	3520	0.7175	-7471B	PPB	03 Mar 2020 12:40:06	U	SMPL
L1743-18 - 1	C-2	14001	2.8078	-7471B	PPB	03 Mar 2020 12:42:24	U	SMPL
L1757-01 - 1	EO-02-030220	2240	0.4622	-7471B	PPB	03 Mar 2020 12:44:39	U	SMPL
CCV45 - 1	CCV45	25833	5.1676	-7471B	PPB	03 Mar 2020 12:46:54	U	SMPL
CCB45 - 1	CCB45	-63	0.0029	-7471B	PPB	03 Mar 2020 12:49:10	U	SMPL
L1762-01 - 1	TR-04-030220	2185	0.4512	-7471B	PPB	03 Mar 2020 12:51:25	U	SMPL
L1762-04 - 1	TR-05-030220	1146	0.2440	-7471B	PPB	03 Mar 2020 12:53:41	U	SMPL
L1762-07 - 1	TR-06-030220	1498	0.3142	-7471B	PPB	03 Mar 2020 12:55:56	U	SMPL
L1763-01 - 1	SOIL	521	0.1194	-7471B	PPB	03 Mar 2020 12:58:12	U	SMPL
L1769-01 - 1	SP-1	1332	0.2811	-7471B	PPB	03 Mar 2020 13:00:27	U	SMPL
L1770-01 - 1	C-1	1826	0.3796	-7471B	PPB	03 Mar 2020 13:02:44	U	SMPL
L1683-22DUP - 1	OF-3-20200225DUP	14079	2.8234	-7471B	PPB	03 Mar 2020 13:05:00	U	SMPL
L1683-23DLX10 - 1		34916	6.9791	-7471B	PPB	03 Mar 2020 13:07:17	U	SMPL
L1683-22LX5 - 1		2633	0.5406	-7471B	PPB	03 Mar 2020 13:09:34	U	SMPL
L1683-22A - 1		33722	6.7410	-7471B	PPB	03 Mar 2020 13:11:50	U	SMPL
CCV46 - 1	CCV46	26195	5.2398	-7471B	PPB	03 Mar 2020 13:14:06	U	SMPL
CCB46 - 1	CCB46	-77	0.0001	-7471B	PPB	03 Mar 2020 13:16:22	U	SMPL