


LB108081

7470A

INSTRUMENT ID: CV1

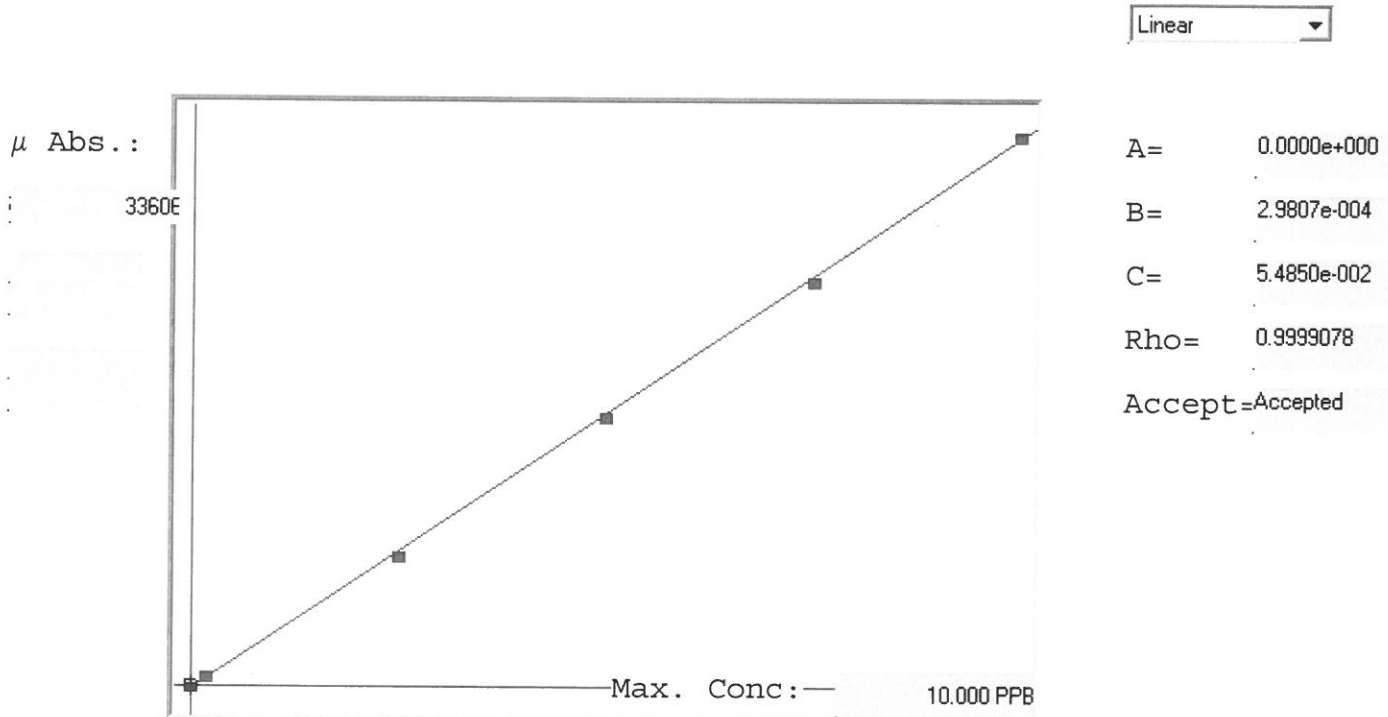

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.040	0.040	-49	0.000	-49				
0.2	0.200	0.233	0.033	599	0.0 %	599				
2.5	2.500	2.450	-0.050	8034	0.0 %	8034				
5.0	5.000	4.960	-0.040	16458	0.0 %	16458				
7.5	7.500	7.445	-0.055	24792	0.0 %	24792				
10.0	10.000	10.072	0.072	33606	0.0 %	33606				

LB108081 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Mar 2020 08:32:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-49	-	0.0000	7470A	PPB	04 Mar 2020 08:40:30	S	Std
0.2 - 1	50.2	599	-	0.2000	7470A	PPB	04 Mar 2020 08:42:37	S	Std
2.5 - 1	52.5	8034	-	2.5000	7470A	PPB	04 Mar 2020 08:44:45	S	Std
5.0 - 1	55	16458	-	5.0000	7470A	PPB	04 Mar 2020 08:46:52	S	Std
7.5 - 1	57.5	24792	-	7.5000	7470A	PPB	04 Mar 2020 08:48:59	S	Std
10.0 - 1	510	33606	-	10.0000	7470A	PPB	04 Mar 2020 08:53:48	S	Std
ICV43 - 1	ICV43	12578	3.8040	-	7470A	PPB	04 Mar 2020 08:56:17	U	SMPL
ICB43 - 1	ICB43	-423	-0.0712	-	7470A	PPB	04 Mar 2020 08:58:24	U	SMPL
CCV49 - 1	CCV49	17041	5.1342	-	7470A	PPB	04 Mar 2020 09:00:32	U	SMPL
CCB49 - 1	CCB49	-426	-0.0721	-	7470A	PPB	04 Mar 2020 09:02:37	U	SMPL
CRA - 1	CRA	517	0.2090	-	7470A	PPB	04 Mar 2020 09:04:44	U	SMPL
HighStd - 1	HighStd	33423	10.0172	-	7470A	PPB	04 Mar 2020 09:06:50	U	SMPL
ChkStd - 1	ChkStd	24138	7.2496	-	7470A	PPB	04 Mar 2020 09:08:56	U	SMPL
PB127246BL - 1	PBW	-156	0.0084	-	7470A	PPB	04 Mar 2020 09:13:42	U	SMPL
PB127246BS - 1	LCSW	12520	3.7867	-	7470A	PPB	04 Mar 2020 09:15:48	U	SMPL
L1757-06 - 1	EO-02-030220	-320	-0.0405	-	7470A	PPB	04 Mar 2020 09:17:55	U	SMPL
L1757-06DUP - 1	EO-02-030220DUP	-101	0.0247	-	7470A	PPB	04 Mar 2020 09:20:03	U	SMPL
L1757-06MS - 1	EO-02-030220MS	12612	3.8141	-	7470A	PPB	04 Mar 2020 09:22:11	U	SMPL
L1757-06MSD - 1	EO-02-030220MSD	12256	3.7080	-	7470A	PPB	04 Mar 2020 09:24:18	U	SMPL
L1762-03 - 1	TR-04-030220	-314	-0.0387	-	7470A	PPB	04 Mar 2020 09:26:25	U	SMPL
CCV50 - 1	CCV50	17423	5.2481	-	7470A	PPB	04 Mar 2020 09:28:32	U	SMPL
CCB50 - 1	CCB50	-403	-0.0653	-	7470A	PPB	04 Mar 2020 09:30:37	U	SMPL
L1762-06 - 1	TR-05-030220	-98	0.0256	-	7470A	PPB	04 Mar 2020 09:32:45	U	SMPL
L1762-09 - 1	TR-06-030220	-54	0.0388	-	7470A	PPB	04 Mar 2020 09:34:51	U	SMPL
L1757-06LX5 - 1		-66	0.0352	-	7470A	PPB	04 Mar 2020 09:36:57	U	SMPL
L1757-06A - 1		12756	3.8570	-	7470A	PPB	04 Mar 2020 09:39:04	U	SMPL
PB127246TB - 1	PB127226TB	-170	0.0042	-	7470A	PPB	04 Mar 2020 09:41:10	U	SMPL
CCV51 - 1	CCV51	17308	5.2138	-	7470A	PPB	04 Mar 2020 09:43:19	U	SMPL
CCB51 - 1	CCB51	-340	-0.0465	-	7470A	PPB	04 Mar 2020 09:45:26	U	SMPL