


LB108106

7470A

INSTRUMENT ID: CV2

 μ Abs.:

33562

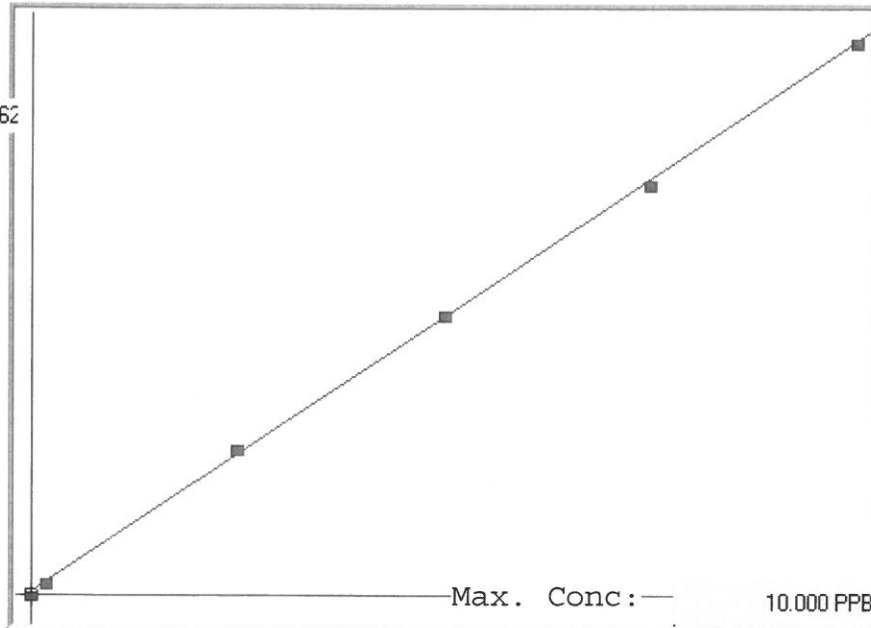

Linear

A= 0.0000e+000

B= 2.9950e-004

C= -5.1339e-002

Rho= 0.9998604

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.059	-0.059	-26	0.000	-26				
0.2	0.200	0.177	-0.023	763	0.0 %	763				
2.5	2.500	2.596	0.096	8840	0.0 %	8840				
5.0	5.000	5.061	0.061	17070	0.0 %	17070				
7.5	7.500	7.424	-0.076	24959	0.0 %	24959				
10.0	10.000	10.001	0.001	33562	0.0 %	33562				

LB108106 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Mar 2020 08:32:40

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-26	-	0.0000	7470A	PPB	05 Mar 2020 08:36:56	S	Std
0.2 - 1	50.2	763	-	0.2000	7470A	PPB	05 Mar 2020 08:39:04	S	Std
2.5 - 1	52.5	8840	-	2.5000	7470A	PPB	05 Mar 2020 08:41:12	S	Std
5.0 - 1	55	17070	-	5.0000	7470A	PPB	05 Mar 2020 08:43:19	S	Std
7.5 - 1	57.5	24959	-	7.5000	7470A	PPB	05 Mar 2020 08:45:26	S	Std
10.0 - 1	57.0	33562	-	10.0000	7470A	PPB	05 Mar 2020 08:50:02	S	Std
ICV45 - 1	ICV45	13620	4.0279	-	7470A	PPB	05 Mar 2020 08:52:34	U	SMPL
ICB45 - 1	ICB45	-51	-0.0666	-	7470A	PPB	05 Mar 2020 08:57:04	U	SMPL
CCV55 - 1	CCV55	17760	5.2678	-	7470A	PPB	05 Mar 2020 08:59:10	U	SMPL
CCB55 - 1	CCB55	20	-0.0453	-	7470A	PPB	05 Mar 2020 09:03:38	U	SMPL
CRA - 1	CRA	849	0.2029	-	7470A	PPB	05 Mar 2020 09:05:44	U	SMPL
HighStd - 1	HighStd	34545	10.2950	-	7470A	PPB	05 Mar 2020 09:07:49	U	SMPL
ChkStd - 1	ChkStd	25377	7.5491	-	7470A	PPB	05 Mar 2020 09:09:55	U	SMPL
PB127269BL - 1	PBW	40	-0.0394	-	7470A	PPB	05 Mar 2020 09:14:28	U	SMPL
PB127269BS - 1	LCSW	13330	3.9410	-	7470A	PPB	05 Mar 2020 09:16:34	U	SMPL
L1721-02 - 1	STOCKPILE-GRIT	1180	0.3021	-	7470A	PPB	05 Mar 2020 09:18:41	U	SMPL
L1748-04 - 1	AU-06-030320	65	-0.0319	-	7470A	PPB	05 Mar 2020 09:20:49	U	SMPL
L1759-05 - 1	OR-02-030320	144	-0.0082	-	7470A	PPB	05 Mar 2020 09:22:58	U	SMPL
L1775-05 - 1	CR-1	380	0.0625	-	7470A	PPB	05 Mar 2020 09:25:05	U	SMPL
L1775-11 - 1	CR-2	340	0.0505	-	7470A	PPB	05 Mar 2020 09:27:11	U	SMPL
CCV56 - 1	CCV56	17673	5.2418	-	7470A	PPB	05 Mar 2020 09:29:17	U	SMPL
CCB56 - 1	CCB56	-58	-0.0687	-	7470A	PPB	05 Mar 2020 09:31:23	U	SMPL
L1775-17 - 1	CR-3	246	0.0223	-	7470A	PPB	05 Mar 2020 09:33:31	U	SMPL
L1775-17DUP - 1	CR-3DUP	226	0.0163	-	7470A	PPB	05 Mar 2020 09:35:37	U	SMPL
L1775-17MS - 1	CR-3MS	12744	3.7655	-	7470A	PPB	05 Mar 2020 09:37:42	U	SMPL
L1775-17MSD - 1	CR-3MSD	13156	3.8889	-	7470A	PPB	05 Mar 2020 09:39:49	U	SMPL
L1775-17LX5 - 1		-161	-0.0996	-	7470A	PPB	05 Mar 2020 09:41:56	U	SMPL
L1775-17A - 1		13959	4.1294	-	7470A	PPB	05 Mar 2020 09:44:03	U	SMPL
PB127269TB - 1	PB127248TB	79	-0.0277	-	7470A	PPB	05 Mar 2020 09:46:10	U	SMPL
CCV57 - 1	CCV57	17710	5.2529	-	7470A	PPB	05 Mar 2020 09:48:18	U	SMPL
CCB57 - 1	CCB57	-139	-0.0930	-	7470A	PPB	05 Mar 2020 09:50:26	U	SMPL