


LB 102122

245.1

INSTRUMENT ID: CV1

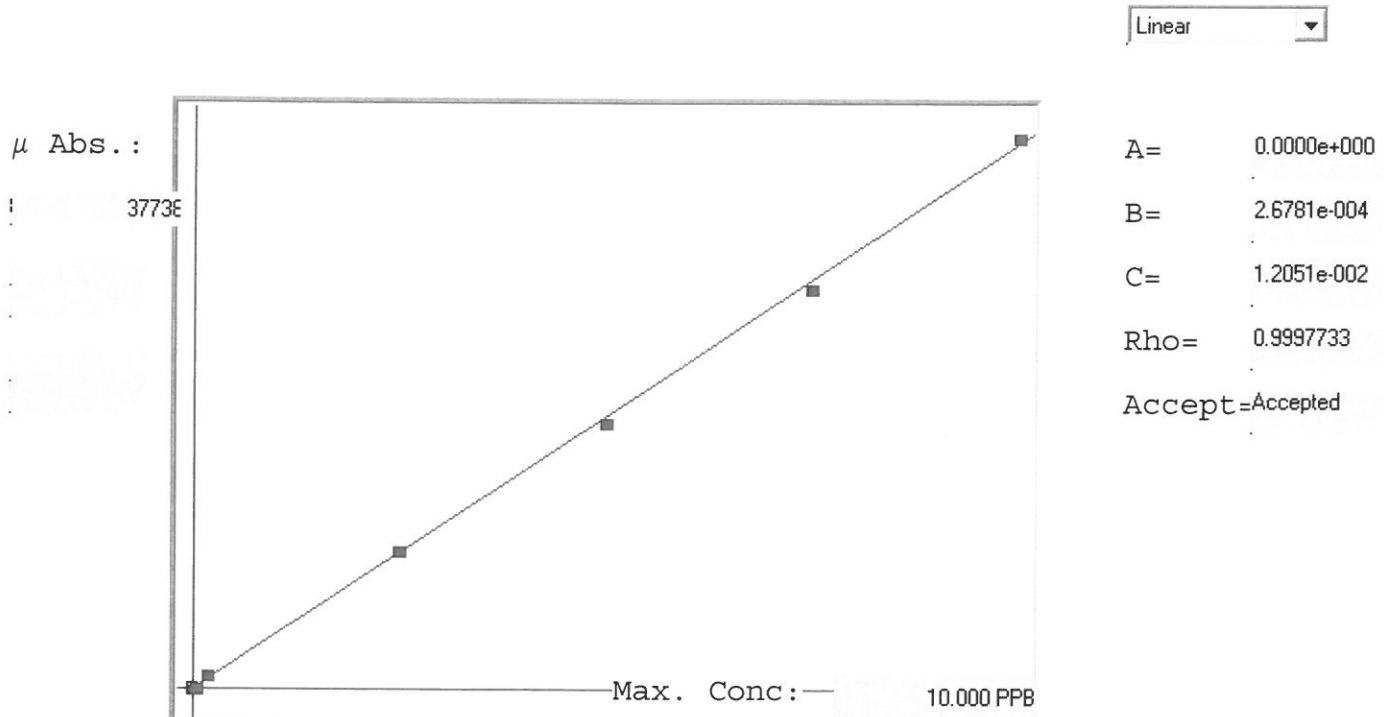

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.015	-0.015	-100	0.000	-100				
0.05	0.050	0.047	-0.003	129	0.0 %	129				
0.2	0.200	0.258	0.058	920	0.0 %	920				
2.5	2.500	2.552	0.052	9485	0.0 %	9485				
5.0	5.000	4.915	-0.085	18309	0.0 %	18309				
7.5	7.500	7.373	-0.127	27486	0.0 %	27486				
10.0	10.000	10.119	0.119	37738	0.0 %	37738				

LB108122 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 05 Mar 2020 14:22:28

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-100	-	0.0000245.1	PPB	05 Mar 2020 14:52:51	S	Std
0.05 - 1	80.05	129	-	0.0500245.1	PPB	05 Mar 2020 14:55:07	S	Std
0.2 - 1	80.2	920	-	0.2000245.1	PPB	05 Mar 2020 14:57:24	S	Std
2.5 - 1	52.5	9485	-	2.5000245.1	PPB	05 Mar 2020 14:59:41	S	Std
5.0 - 1	55	18309	-	5.0000245.1	PPB	05 Mar 2020 15:01:57	S	Std
7.5 - 1	57.5	27486	-	7.5000245.1	PPB	05 Mar 2020 15:04:13	S	Std
10.0 - 1	81.6	37738	-	10.0000245.1	PPB	05 Mar 2020 15:09:11	S	Std
ICV47 - 1	ICV47	14264	3.8321	-245.1	PPB	05 Mar 2020 15:17:09	U	SMPL
ICB47 - 1	ICB47	-290	-0.0656	-245.1	PPB	05 Mar 2020 15:19:24	U	SMPL
CCV64 - 1	CCV64	18737	5.0301	-245.1	PPB	05 Mar 2020 15:21:40	U	SMPL
CCB64 - 1	CCB64	-187	-0.0380	-245.1	PPB	05 Mar 2020 15:23:54	U	SMPL
CRA - 1	CRA	153	0.0530	-245.1	PPB	05 Mar 2020 15:26:10	U	SMPL
HighStd - 1	HighStd	37540	10.0658	-245.1	PPB	05 Mar 2020 15:28:25	U	SMPL
ChkStd - 1	ChkStd	25556	6.8563	-245.1	PPB	05 Mar 2020 15:30:40	U	SMPL
PB127297BL - 1	PBW	-320	-0.0736	-245.1	PPB	05 Mar 2020 15:32:58	U	SMPL
PB127297BS - 1	LCSW	14119	3.7933	-245.1	PPB	05 Mar 2020 15:35:15	U	SMPL
L1161-12 - 1	MDL-WATER-06-QT1-2020	135	0.0482	-245.1	PPB	05 Mar 2020 15:40:40	U	SMPL
L1796-01 - 1	COMP	327	0.0996	-245.1	PPB	05 Mar 2020 15:47:54	U	SMPL
L1796-01DUP - 1	COMPDUP	284	0.0881	-245.1	PPB	05 Mar 2020 15:50:10	U	SMPL
L1796-01MS - 1	COMPMS	15019	4.0343	-245.1	PPB	05 Mar 2020 15:58:04	U	SMPL
L1796-01MSD - 1	COMPMSD	14695	3.9476	-245.1	PPB	05 Mar 2020 16:00:19	U	SMPL
CCV65 - 1	CCV65	18071	4.8517	-245.1	PPB	05 Mar 2020 16:02:35	U	SMPL
CCB65 - 1	CCB65	-191	-0.0391	-245.1	PPB	05 Mar 2020 16:04:50	U	SMPL
L1796-01LX5 - 1		107	0.0407	-245.1	PPB	05 Mar 2020 16:07:06	U	SMPL
L1796-01A - 1		14400	3.8686	-245.1	PPB	05 Mar 2020 16:09:22	U	SMPL
CCV66 - 1	CCV66	18324	4.9195	-245.1	PPB	05 Mar 2020 16:11:37	U	SMPL
CCB66 - 1	CCB66	-154	-0.0292	-245.1	PPB	05 Mar 2020 16:13:53	U	SMPL