

LB 108153


7470A

INSTRUMENT ID: CY1

Linear

 μ Abs.:

36756

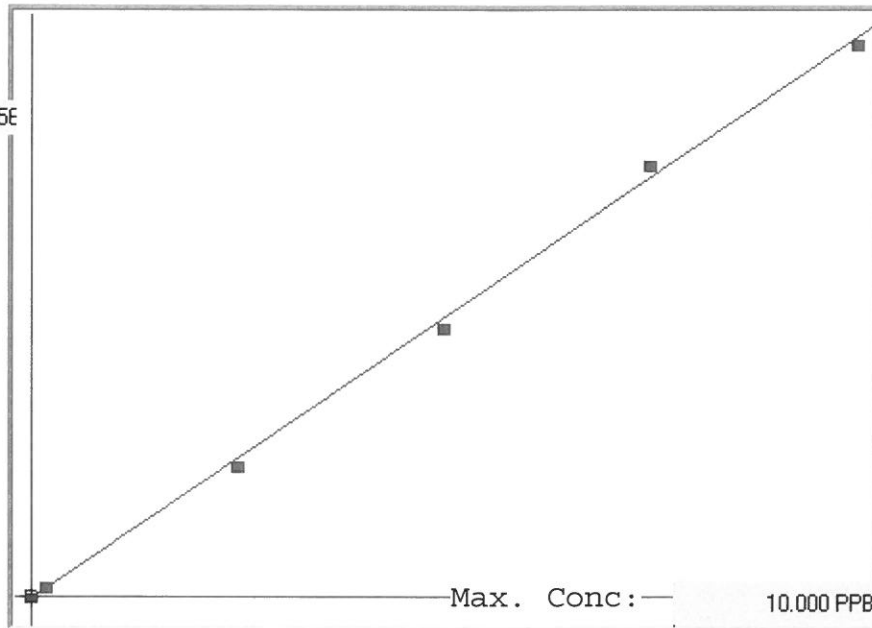

A= 0.0000e+000

B= 2.6832e-004

C= 5.0935e-002

Rho= 0.9993948

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.054	0.054	12	0.000	12				
0.2	0.200	0.247	0.047	732	0.0 %	732				
2.5	2.500	2.400	-0.100	8754	0.0 %	8754				
5.0	5.000	4.852	-0.148	17895	0.0 %	17895				
7.5	7.500	7.733	0.233	28631	0.0 %	28631				
10.0	10.000	9.913	-0.087	36756	0.0 %	36756				

LB108153 INSTRUMENT ID ; CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Mar 2020 13:54:54

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc.	Method	Units	Date	Type	Type
0.0 - 1	50	12	-	0.0000	7470A	PPB	06 Mar 2020 14:06:12	S	Std
0.2 - 1	3020	732	-	0.2000	7470A	PPB	06 Mar 2020 14:08:19	S	Std
2.5 - 1	52.5	8754	-	2.5000	7470A	PPB	06 Mar 2020 14:10:27	S	Std
5.0 - 1	55	17895	-	5.0000	7470A	PPB	06 Mar 2020 14:12:35	S	Std
7.5 - 1	59.5	28631	-	7.5000	7470A	PPB	06 Mar 2020 14:14:42	S	Std
10.0 - 1	510	36756	-	10.0000	7470A	PPB	06 Mar 2020 14:19:21	S	Std
ICV49 - 1	ICV49	13869	3.7722	-	7470A	PPB	06 Mar 2020 14:22:01	U	SMPL
ICB49 - 1	ICB49	-236	-0.0124	-	7470A	PPB	06 Mar 2020 14:24:06	U	SMPL
CCV72 - 1	CCV72	17716	4.8044	-	7470A	PPB	06 Mar 2020 14:26:12	U	SMPL
CCB72 - 1	CCB72	-226	-0.0097	-	7470A	PPB	06 Mar 2020 14:28:18	U	SMPL
CRA - 1	CRA	676	0.2323	-	7470A	PPB	06 Mar 2020 14:30:24	U	SMPL
HighStd - 1	HighStd	36353	9.8050	-	7470A	PPB	06 Mar 2020 14:32:29	U	SMPL
ChkStd - 1	ChkStd	25989	7.0242	-	7470A	PPB	06 Mar 2020 14:34:35	U	SMPL
PB127329BL - 1	PBW	-294	-0.0279	-	7470A	PPB	06 Mar 2020 14:36:43	U	SMPL
PB127329BS - 1	LCSW	14410	3.9174	-	7470A	PPB	06 Mar 2020 14:38:51	U	SMPL
L1803-01 - 1	N38129	156	0.0928	-	7470A	PPB	06 Mar 2020 14:45:54	U	SMPL
L1803-01DUP - 1	N38129DUP	161	0.0941	-	7470A	PPB	06 Mar 2020 14:48:01	U	SMPL
L1803-01MS - 1	N38129MS	15615	4.2407	-	7470A	PPB	06 Mar 2020 14:50:08	U	SMPL
L1803-01MSD - 1	N38129MSD	15773	4.2831	-	7470A	PPB	06 Mar 2020 14:52:14	U	SMPL
CCV73 - 1	CCV73	17655	4.7881	-	7470A	PPB	06 Mar 2020 14:54:21	U	SMPL
CCB73 - 1	CCB73	-162	0.0075	-	7470A	PPB	06 Mar 2020 14:56:26	U	SMPL
PB127330BL - 1	PBW	-41	0.0399	-	7470A	PPB	06 Mar 2020 14:58:33	U	SMPL
PB127330BS - 1	LCSW	12843	3.4969	-	7470A	PPB	06 Mar 2020 15:00:39	U	SMPL
L1366-01 - 1	03-05-A	-171	0.0051	-	7470A	PPB	06 Mar 2020 15:02:45	U	SMPL
L1366-02 - 1	03-05-B	-42	0.0397	-	7470A	PPB	06 Mar 2020 15:04:52	U	SMPL
L1366-03 - 1	03-05-C	-34	0.0418	-	7470A	PPB	06 Mar 2020 15:06:58	U	SMPL
L1366-04 - 1	03-05-D	-7	0.0491	-	7470A	PPB	06 Mar 2020 15:09:05	U	SMPL
L1366-05 - 1	03-05-E	30	0.0590	-	7470A	PPB	06 Mar 2020 15:11:12	U	SMPL
L1366-06 - 1	03-05-F	-3	0.0501	-	7470A	PPB	06 Mar 2020 15:13:20	U	SMPL
L1366-07 - 1	03-05-G	-1	0.0507	-	7470A	PPB	06 Mar 2020 15:15:28	U	SMPL
L1366-08 - 1	03-05-H	-9	0.0485	-	7470A	PPB	06 Mar 2020 15:17:34	U	SMPL
CCV74 - 1	CCV74	17517	4.7510	-	7470A	PPB	06 Mar 2020 15:19:40	U	SMPL
CCB74 - 1	CCB74	-171	0.0051	-	7470A	PPB	06 Mar 2020 15:21:46	U	SMPL
L1366-09 - 1	03-05-I	-35	0.0415	-	7470A	PPB	06 Mar 2020 15:23:53	U	SMPL
L1366-10 - 1	03-05-J	-5	0.0496	-	7470A	PPB	06 Mar 2020 15:25:59	U	SMPL
L1366-11 - 1	03-05-K	-1	0.0507	-	7470A	PPB	06 Mar 2020 15:28:05	U	SMPL
L1366-12 - 1	03-05-OD	-2	0.0504	-	7470A	PPB	06 Mar 2020 15:30:11	U	SMPL
L1753-08 - 1	CL-01-030520	-6	0.0493	-	7470A	PPB	06 Mar 2020 15:32:18	U	SMPL
L1761-05 - 1	SU-04-030420	-2	0.0504	-	7470A	PPB	06 Mar 2020 15:34:25	U	SMPL
L1762-12 - 1	TR-08-030520	15	0.0550	-	7470A	PPB	06 Mar 2020 15:36:32	U	SMPL
L1762-12DUP - 1	TR-08-030520DUP	7	0.0528	-	7470A	PPB	06 Mar 2020 15:38:40	U	SMPL
L1762-12MS - 1	TR-08-030520MS	14478	3.9356	-	7470A	PPB	06 Mar 2020 15:40:47	U	SMPL
L1762-12MSD - 1	TR-08-030520MSD	14932	4.0574	-	7470A	PPB	06 Mar 2020 15:42:53	U	SMPL
CCV75 - 1	CCV75	18013	4.8841	-	7470A	PPB	06 Mar 2020 15:44:59	U	SMPL
CCB75 - 1	CCB75	-195	-0.0014	-	7470A	PPB	06 Mar 2020 15:47:06	U	SMPL
L1791-01 - 1	03-04-A	-42	0.0397	-	7470A	PPB	06 Mar 2020 15:49:12	U	SMPL
L1791-02 - 1	03-04-B	-16	0.0466	-	7470A	PPB	06 Mar 2020 15:51:18	U	SMPL
L1791-03 - 1	03-04-C	-8	0.0488	-	7470A	PPB	06 Mar 2020 15:53:24	U	SMPL
L1791-04 - 1	03-04-D	-19	0.0458	-	7470A	PPB	06 Mar 2020 15:55:30	U	SMPL
L1800-07 - 1	PT-HG-WP	91637	24.6386	-	7470A	PPB	06 Mar 2020 15:59:44	U	SMPL
L1803-01LX5 - 1		-196	-0.0017	-	7470A	PPB	06 Mar 2020 16:06:35	U	SMPL
L1803-01A - 1		15238	4.1395	-	7470A	PPB	06 Mar 2020 16:08:40	U	SMPL
L1762-12LX5 - 1		-170	0.0053	-	7470A	PPB	06 Mar 2020 16:10:47	U	SMPL
L1762-12A - 1		14524	3.9480	-	7470A	PPB	06 Mar 2020 16:12:53	U	SMPL
CCV76 - 1	CCV76	17592	4.7712	-	7470A	PPB	06 Mar 2020 16:14:59	U	SMPL
CCB76 - 1	CCB76	-245	-0.0148	-	7470A	PPB	06 Mar 2020 16:17:06	U	SMPL
L1800-07DLX5 - 1	PT-HG-WP	17741	4.8111	-	7470A	PPB	06 Mar 2020 16:27:44	U	SMPL
PB127330TB - 1	PB127295TB	-185	0.0013	-	7470A	PPB	06 Mar 2020 16:29:51	U	SMPL
CCV77 - 1	CCV77	17702	4.8007	-	7470A	PPB	06 Mar 2020 16:32:00	U	SMPL
CCB77 - 1	CCB77	-241	-0.0137	-	7470A	PPB	06 Mar 2020 16:34:07	U	SMPL