


LB100169

245.1

INSTRUMENT ID : CV1

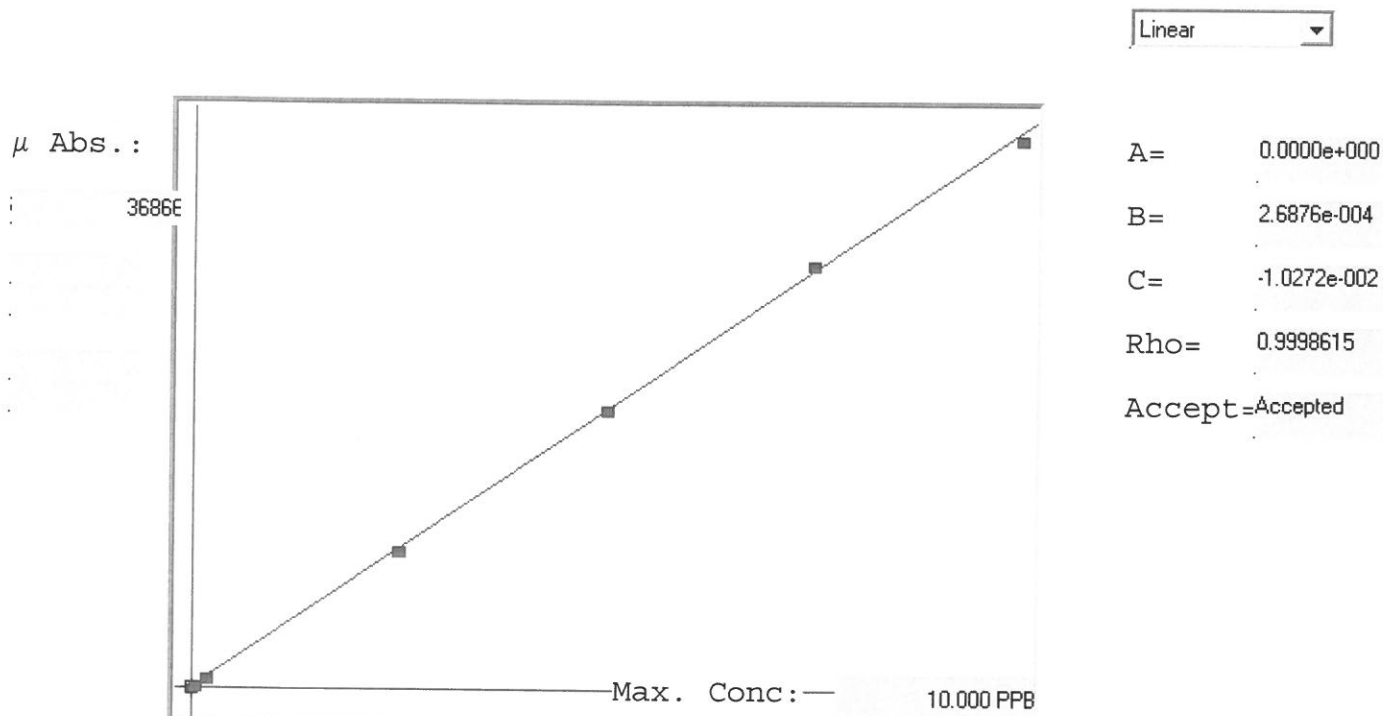

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.016	-0.016	-23	0.000	-23				
0.05	0.050	0.050	-0.000	223	0.0 %	223				
0.2	0.200	0.190	-0.010	747	0.0 %	747				
2.5	2.500	2.479	-0.021	9261	0.0 %	9261				
5.0	5.000	5.029	0.029	18751	0.0 %	18751				
7.5	7.500	7.621	0.121	28394	0.0 %	28394				
10.0	10.000	9.898	-0.102	36866	0.0 %	36866				

LB108169 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 06 Mar 2020 16:50:27

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-23	-	0.0000	245.1	PPB	06 Mar 2020 16:51:18	S	Std
0.05 - 1	50.05	223	-	0.0500	245.1	PPB	06 Mar 2020 16:53:35	S	Std
0.2 - 1	50.2	747	-	0.2000	245.1	PPB	06 Mar 2020 16:55:52	S	Std
2.5 - 1	52.5	9261	-	2.5000	245.1	PPB	06 Mar 2020 16:58:09	S	Std
5.0 - 1	55	18751	-	5.0000	245.1	PPB	06 Mar 2020 17:00:25	S	Std
7.5 - 1	57.5	28394	-	7.5000	245.1	PPB	06 Mar 2020 17:02:41	S	Std
10.0 - 1	510	36866	-	10.0000	245.1	PPB	06 Mar 2020 17:12:39	S	Std
ICV50 - 1	ICV50	14639	3.9240	-245.1		PPB	06 Mar 2020 17:18:04	U	SMPL
ICB50 - 1	ICB50	-198	-0.0635	-245.1		PPB	06 Mar 2020 17:20:18	U	SMPL
CCV78 - 1	CCV78	18789	5.0394	-245.1		PPB	06 Mar 2020 17:22:33	U	SMPL
CCB78 - 1	CCB78	-144	-0.0490	-245.1		PPB	06 Mar 2020 17:24:48	U	SMPL
CRA - 1	CRA	189	0.0405	-245.1		PPB	06 Mar 2020 17:29:35	U	SMPL
HighStd - 1	HighStd	36547	9.8119	-245.1		PPB	06 Mar 2020 17:31:50	U	SMPL
ChkStd - 1	ChkStd	27149	7.2862	-245.1		PPB	06 Mar 2020 17:34:05	U	SMPL
PB127328BL - 1	PBW	-56	-0.0253	-245.1		PPB	06 Mar 2020 17:38:55	U	SMPL
PB127328BS - 1	LCSW	14723	3.9466	-245.1		PPB	06 Mar 2020 17:41:11	U	SMPL
L1799-08 - 1	PT-HG-WP	91841	24.6725	-245.1		PPB	06 Mar 2020 17:43:27	U	SMPL
L1814-01 - 1	15220012-1	183	0.0389	-245.1		PPB	06 Mar 2020 17:45:43	U	SMPL
L1814-01DUP - 1	15220012-1DUP	61	0.0061	-245.1		PPB	06 Mar 2020 17:48:03	U	SMPL
L1814-01MS - 1	15220012-1MS	13024	3.4900	-245.1		PPB	06 Mar 2020 17:50:20	U	SMPL
L1814-01MSD - 1	15220012-1MSD	13702	3.6722	-245.1		PPB	06 Mar 2020 17:52:35	U	SMPL
CCV79 - 1	CCV79	18965	5.0867	-245.1		PPB	06 Mar 2020 17:54:51	U	SMPL
CCB79 - 1	CCB79	-130	-0.0452	-245.1		PPB	06 Mar 2020 17:57:07	U	SMPL
L1815-01 - 1	32220008-3	-47	-0.0229	-245.1		PPB	06 Mar 2020 17:59:23	U	SMPL
L1814-01LX5 - 1		26	-0.0033	-245.1		PPB	06 Mar 2020 18:11:12	U	SMPL
L1814-01A - 1		14248	3.8190	-245.1		PPB	06 Mar 2020 18:13:27	U	SMPL
CCV80 - 1	CCV80	18742	5.0267	-245.1		PPB	06 Mar 2020 18:15:43	U	SMPL
CCB80 - 1	CCB80	-171	-0.0562	-245.1		PPB	06 Mar 2020 18:18:00	U	SMPL
L1799-08DLX5 - 1	PT-HG-WP	18728	5.0230	-245.1		PPB	06 Mar 2020 18:20:18	U	SMPL
CCV81 - 1	CCV81	19070	5.1149	-245.1		PPB	06 Mar 2020 18:27:06	U	SMPL
CCB81 - 1	CCB81	-172	-0.0565	-245.1		PPB	06 Mar 2020 18:29:22	U	SMPL