

LB108226

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : JK

Instrument ID : Konelab

3/11/2020 12:27

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.947	0.0	0.090	
ICB1	0.460	0.0	0.003	
CCV1	245.898	0.0	0.223	
CCB1	0.182	0.0	0.003	
PB127334BL	0.216	0.0	0.003	
PB127334BS	98.381	0.0	0.091	
LOWPB127334	9.920	0.0	0.012	
HIGHPB127334	494.069	0.0	0.446	
L1801-25	594.522	0.0	0.536	Test limit high
L1801-25DLX2	294.317	0.0	0.267	
CCV2	246.592	0.0	0.224	
CCB2	0.237	0.0	0.003	

N	12
Mean	173.479
SD	205.2706
CV%	118.33

LB108226

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 11 12:23:25 2020

Wed Mar 11 12:26:13 2020

Dk

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.3	µg/l	3/11/2020 10:19:37	
5.OPPBCN	A	Total CN	P	4.4557	µg/l	3/11/2020 10:19:38	
10PPBCN	A	Total CN	P	9.2339	µg/l	3/11/2020 10:19:39	
50PPBCN	A	Total CN	P	50.1681	µg/l	3/11/2020 10:19:40	
100PPBCN	A	Total CN	P	100.0444	µg/l	3/11/2020 10:19:41	
250PPBCN	A	Total CN	P	252.8057	µg/l	3/11/2020 10:19:42	
500PPBCN	A	Total CN	P	498.5922	µg/l	3/11/2020 10:19:43	
ICV1	S	Total CN	P	96.9473	µg/l	3/11/2020 12:23:25	
ICB1	S	Total CN	P	0.4599	µg/l	3/11/2020 12:23:26	
CCV1	S	Total CN	P	245.8978	µg/l	3/11/2020 12:23:27	
CCB1	S	Total CN	P	0.1822	µg/l	3/11/2020 12:23:28	
PB127334BL	S	Total CN	P	0.2164	µg/l	3/11/2020 12:23:29	
PB127334BS	S	Total CN	P	98.3809	µg/l	3/11/2020 12:23:30	
LOWPB127334	S	Total CN	P	9.92	µg/l	3/11/2020 12:23:31	
HIGHPB127334	S	Total CN	P	494.0691	µg/l	3/11/2020 12:23:32	
L1801-25	S	Total CN	P	594.5225	µg/l	3/11/2020 12:23:33	
L1801-25DLX2	S	Total CN	P	294.3171	µg/l	3/11/2020 12:23:34	
CCV2	S	Total CN	P	246.5921	µg/l	3/11/2020 12:23:35	
CCB2	S	Total CN	P	0.2368	µg/l	3/11/2020 12:26:13	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Du

Instrument ID : Konelab

3/11/2020 17:11


Test Total CN

Accepted 3/11/2020 10:24

Factor 1115
Bias 0.003

Coeff. of det. 0.999947

Errors

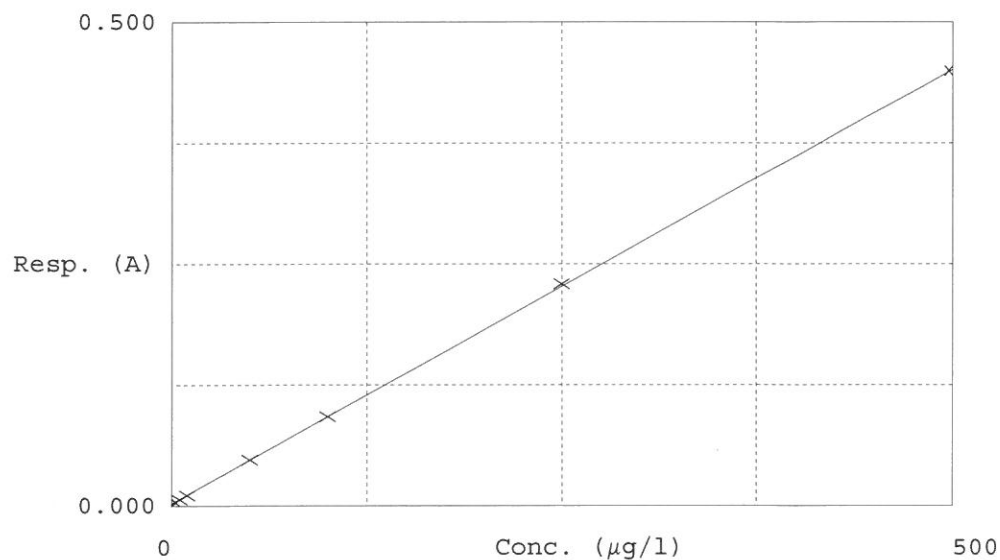

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.3000	0.0000	
2	5.0PPBCN	0.007	4.4557	5.0000	
3	10PPBCN	0.011	9.2339	10.0000	
4	50PPBCN	0.048	50.1681	50.0000	
5	100PPBCN	0.092	100.0444	100.0000	
6	250PPBCN	0.229	252.8057	250.0000	
7	500PPBCN	0.450	498.5922	500.0000	