


LB108449

7471B

INSTRUMENT ID: CV1

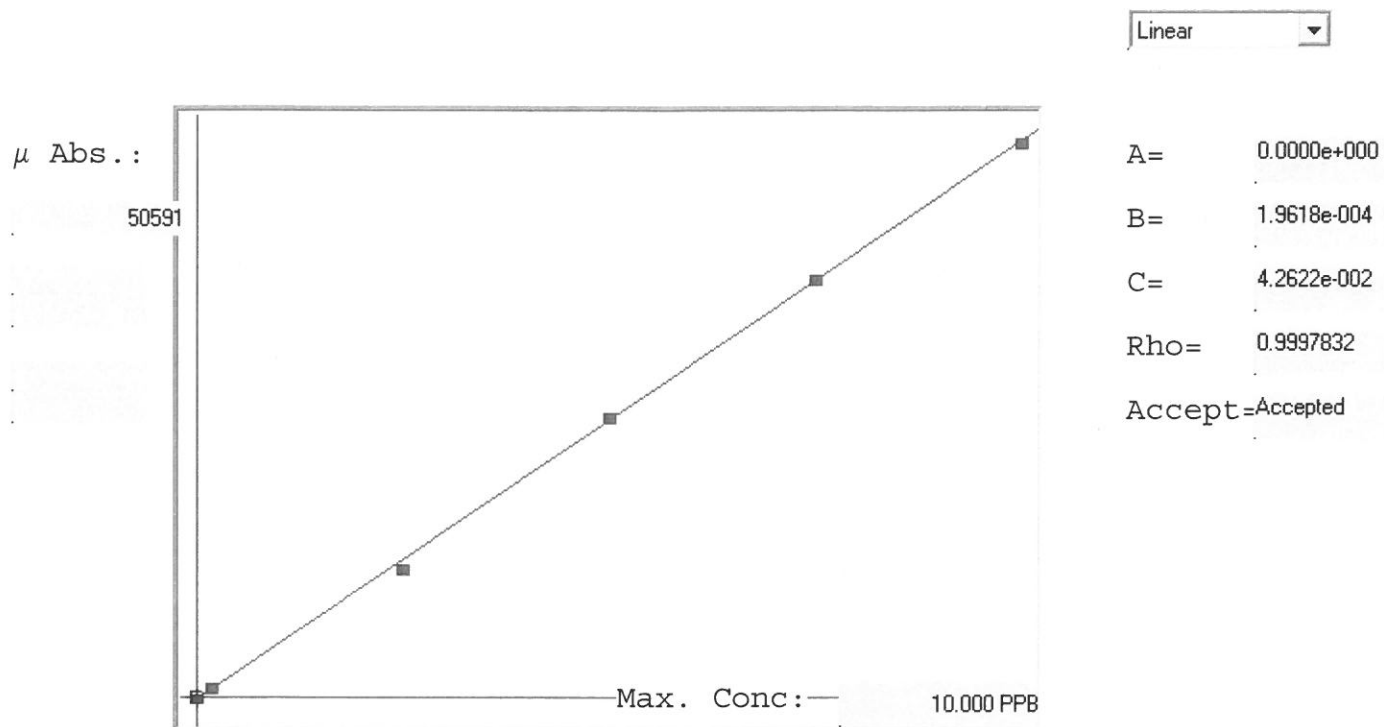

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.049	0.049	32	0.000	32				
0.2	0.200	0.218	0.018	895	0.0 %	895				
2.5	2.500	2.348	-0.152	11750	0.0 %	11750				
5.0	5.000	5.086	0.086	25710	0.0 %	25710				
7.5	7.500	7.531	0.031	38174	0.0 %	38174				
10.0	10.000	9.967	-0.033	50591	0.0 %	50591				

LB108449 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 26 Mar 2020 08:53:35

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	32	-	0.00007471B	PPB	26 Mar 2020 08:58:31	S	Std
0.2 - 1	50.2	895	-	0.20007471B	PPB	26 Mar 2020 09:00:48	S	Std
2.5 - 1	52.5	11750	-	2.50007471B	PPB	26 Mar 2020 09:03:05	S	Std
5.0 - 1	55	25710	-	5.00007471B	PPB	26 Mar 2020 09:05:22	S	Std
7.5 - 1	57.5	38174	-	7.50007471B	PPB	26 Mar 2020 09:07:39	S	Std
10.0 - 1	510	50591	-	10.00007471B	PPB	26 Mar 2020 09:09:56	S	Std
ICV77 - 1	ICV77	18559	3.6835	-7471B	PPB	26 Mar 2020 09:12:43	U	SMPL
ICB77 - 1	ICB77	-210	0.0014	-7471B	PPB	26 Mar 2020 09:15:00	U	SMPL
CCV01 - 1	CCV01	26618	5.2645	-7471B	PPB	26 Mar 2020 09:17:16	U	SMPL
CCB01 - 1	CCB01	-231	-0.0027	-7471B	PPB	26 Mar 2020 09:19:31	U	SMPL
CRA - 1	CRA	873	0.2139	-7471B	PPB	26 Mar 2020 09:21:47	U	SMPL
HighStd - 1	HighStd	51325	10.1114	-7471B	PPB	26 Mar 2020 09:24:02	U	SMPL
ChkStd - 1	ChkStd	34683	6.8466	-7471B	PPB	26 Mar 2020 09:26:17	U	SMPL
PB127819BL - 1	PBS	-336	-0.0233	-7471B	PPB	26 Mar 2020 09:28:35	U	SMPL
PB127819BS - 1	LCSS	20052	3.9764	-7471B	PPB	26 Mar 2020 09:30:52	U	SMPL
L1753-09 - 1	CL-02-032520	4011	0.8295	-7471B	PPB	26 Mar 2020 09:33:08	U	SMPL
L1761-11 - 1	SU-02-032520	6184	1.2558	-7471B	PPB	26 Mar 2020 09:35:26	U	SMPL
L2009-01 - 1	TRACKS-66-67	3520	0.7332	-7471B	PPB	26 Mar 2020 09:37:44	U	SMPL
L2032-01 - 1	SOIL-CUTTINGS-1	186	0.0791	-7471B	PPB	26 Mar 2020 09:40:00	U	SMPL
L2034-01 - 1	FK-BPM-04-008-ABCD	1150	0.2682	-7471B	PPB	26 Mar 2020 09:45:09	U	SMPL
CCV02 - 1	CCV02	27024	5.3441	-7471B	PPB	26 Mar 2020 09:47:24	U	SMPL
CCB02 - 1	CCB02	-105	0.0220	-7471B	PPB	26 Mar 2020 09:49:39	U	SMPL
L2034-01DUP - 1	FK-BPM-04-008-ABCDDUP	1373	0.3120	-7471B	PPB	26 Mar 2020 09:51:55	U	SMPL
L2034-01MS - 1	FK-BPM-04-008-ABCDMS	24154	4.7811	-7471B	PPB	26 Mar 2020 09:54:10	U	SMPL
L2034-01MSD - 1	FK-BPM-04-008-ABCDMSD	21393	4.2394	-7471B	PPB	26 Mar 2020 09:56:25	U	SMPL
L2035-01 - 1	FK-GF-02-054-A	4904	1.0047	-7471B	PPB	26 Mar 2020 09:58:42	U	SMPL
L2035-03 - 1	FK-GF-02-054-B	6476	1.3131	-7471B	PPB	26 Mar 2020 10:00:58	U	SMPL
L2036-01 - 1	FK-BPM-03-014-ABCD	1723	0.3806	-7471B	PPB	26 Mar 2020 10:03:14	U	SMPL
L2037-01 - 1	FK-BPM-01-C4-D4-C4A-D4A	1236	0.2851	-7471B	PPB	26 Mar 2020 10:05:30	U	SMPL
L2040-01 - 1	RO-350	22141	4.3862	-7471B	PPB	26 Mar 2020 10:07:47	U	SMPL
L2040-04 - 1	RO-06	3232	0.6767	-7471B	PPB	26 Mar 2020 10:10:03	U	SMPL
L2040-07 - 1	RO-11986	3178	0.6661	-7471B	PPB	26 Mar 2020 10:12:20	U	SMPL
CCV03 - 1	CCV03	26642	5.2692	-7471B	PPB	26 Mar 2020 10:14:35	U	SMPL
CCB03 - 1	CCB03	-86	0.0258	-7471B	PPB	26 Mar 2020 10:16:51	U	SMPL
L2040-10 - 1	RO-346	3101	0.6510	-7471B	PPB	26 Mar 2020 10:19:07	U	SMPL
L2040-13 - 1	RO-209	5254	1.0733	-7471B	PPB	26 Mar 2020 10:21:22	U	SMPL
L2042-03 - 1	SB-03-5.5-6.0	1923	0.4199	-7471B	PPB	26 Mar 2020 10:23:37	U	SMPL
L2042-04 - 1	SB-04-5.5-6.0	2893	0.6102	-7471B	PPB	26 Mar 2020 10:25:53	U	SMPL
L2043-02 - 1	TP-2A	835	0.2064	-7471B	PPB	26 Mar 2020 10:28:09	U	SMPL
L2043-06 - 1	TP-1A	380	0.1172	-7471B	PPB	26 Mar 2020 10:30:25	U	SMPL
L2034-01LX5 - 1		290	0.0995	-7471B	PPB	26 Mar 2020 10:32:41	U	SMPL
L2034-01A - 1		23210	4.5959	-7471B	PPB	26 Mar 2020 10:34:58	U	SMPL
CCV04 - 1	CCV04	24702	4.8886	-7471B	PPB	26 Mar 2020 10:37:15	U	SMPL
CCB04 - 1	CCB04	-77	0.0275	-7471B	PPB	26 Mar 2020 10:39:30	U	SMPL