

LB108480

Result archive

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : De

Instrument ID : Konelab

3/27/2020 13:02

mg/L

Sample id	Test id	Result	Status	Date	Errors
<i>De</i> <i>3/27/20</i> ICV1	Total CN	96.067	man acc	3/27/2020	
ICV1	Total CN	96.835	man acc	3/27/2020	
ICB1	Total CN	-1.013	man acc	3/27/2020	
CCV1	Total CN	248.235	man acc	3/27/2020	
CCB1	Total CN	-1.201	man acc	3/27/2020	
PB127871BL	Total CN	-1.227	man acc	3/27/2020	
L2049-05	Total CN	-1.269	man acc	3/27/2020	
L2049-05DUP	Total CN	-0.866	man acc	3/27/2020	
L2053-04	Total CN	-1.096	man acc	3/27/2020	
L2053-08	Total CN	-1.359	man acc	3/27/2020	
L2055-05	Total CN	-1.193	man acc	3/27/2020	
PB127873BL	Total CN	-0.509	man acc	3/27/2020	
L2053-11	Total CN	-1.346	man acc	3/27/2020	
L2053-11DUP	Total CN	1.378	man acc	3/27/2020	Blank resp. hig
L1754-04	Total CN	-1.144	man acc	3/27/2020	
CCV2	Total CN	245.266	man acc	3/27/2020	
CCB2	Total CN	-1.373	man acc	3/27/2020	

Aquakem v. 7.2AQ1

Results from time period:

Fri Mar 27 12:06:50 2020

Fri Mar 27 12:54:00 2020

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	-1.3405	µg/l	3/27/2020 12:06:50
5.OPPBCN	A	REACTIVE CN	P	3.8986	µg/l	3/27/2020 12:06:51
10PPBCN	A	REACTIVE CN	P	8.9773	µg/l	3/27/2020 12:06:52
50PPBCN	A	REACTIVE CN	P	49.6012	µg/l	3/27/2020 12:06:53
100PPBCN	A	REACTIVE CN	P	100.5995	µg/l	3/27/2020 12:06:54
250PPBCN	A	REACTIVE CN	P	256.6249	µg/l	3/27/2020 12:06:55
500PPBCN	A	REACTIVE CN	P	496.639	µg/l	3/27/2020 12:06:56
ICV1	S	REACTIVE CN	P	96.835	µg/l	3/27/2020 12:43:02
ICB1	S	REACTIVE CN	P	-1.013	µg/l	3/27/2020 12:43:03
CCV1	S	REACTIVE CN	P	248.2354	µg/l	3/27/2020 12:43:06
CCB1	S	REACTIVE CN	P	-1.2009	µg/l	3/27/2020 12:43:08
PB127871BL	S	REACTIVE CN	P	-1.2274	µg/l	3/27/2020 12:43:09
L2049-05	S	REACTIVE CN	P	-1.2685	µg/l	3/27/2020 12:43:11
L2049-05DUP	S	REACTIVE CN	P	-0.8655	µg/l	3/27/2020 12:50:36
L2053-04	S	REACTIVE CN	P	-1.0961	µg/l	3/27/2020 12:50:37
L2053-08	S	REACTIVE CN	P	-1.3588	µg/l	3/27/2020 12:50:38
L2055-05	S	REACTIVE CN	P	-1.1929	µg/l	3/27/2020 12:50:39
PB127873BL	S	REACTIVE CN	P	-0.509	µg/l	3/27/2020 12:50:40
L2053-11	S	REACTIVE CN	P	-1.346	µg/l	3/27/2020 12:50:42
L2053-11DUP	S	REACTIVE CN	P	1.3778	µg/l	3/27/2020 12:50:43
L1754-04	S	REACTIVE CN	P	-1.1437	µg/l	3/27/2020 12:50:44
CCV2	S	REACTIVE CN	P	245.2655	µg/l	3/27/2020 12:50:45
CCB2	S	REACTIVE CN	P	-1.3735	µg/l	3/27/2020 12:54:00

LB108480

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : De

Instrument ID : Konelab

3/27/2020 12:09


Test ~~Total~~ ^{perme} CN

Accepted 3/27/2020 12:09

Factor 1084
Bias 0.004

Coeff. of det. 0.999709

Errors

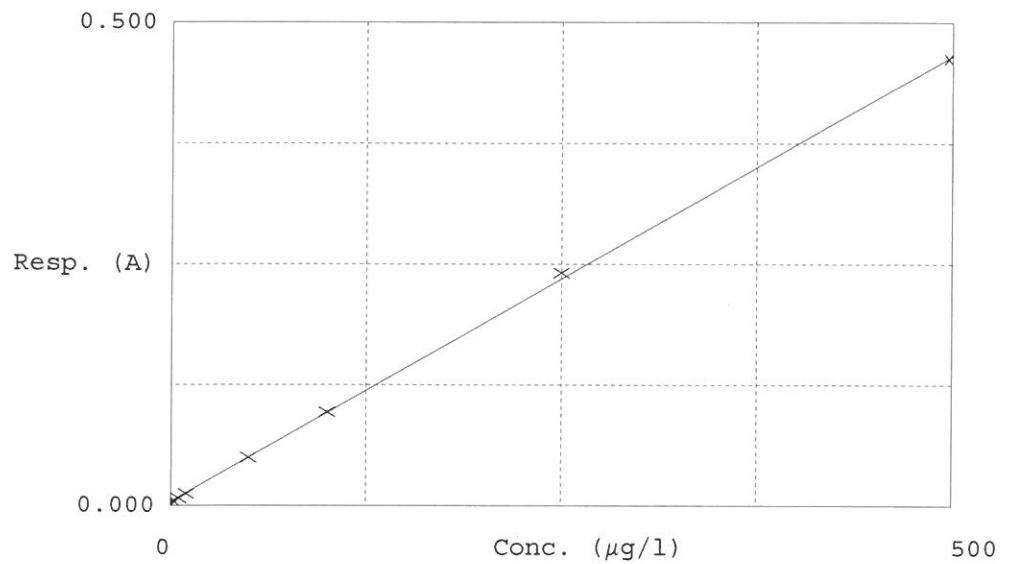

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.3405	0.0000	
2	5.0PPBCN	0.008	3.8986	5.0000	
3	10PPBCN	0.012	8.9773	10.0000	
4	50PPBCN	0.050	49.6012	50.0000	
5	100PPBCN	0.097	100.5995	100.0000	
6	250PPBCN	0.241	256.6249	250.0000	
7	500PPBCN	0.462	496.6390	500.0000	