


LB108531

7470A

INSTRUMENT ID: CV1

Linear

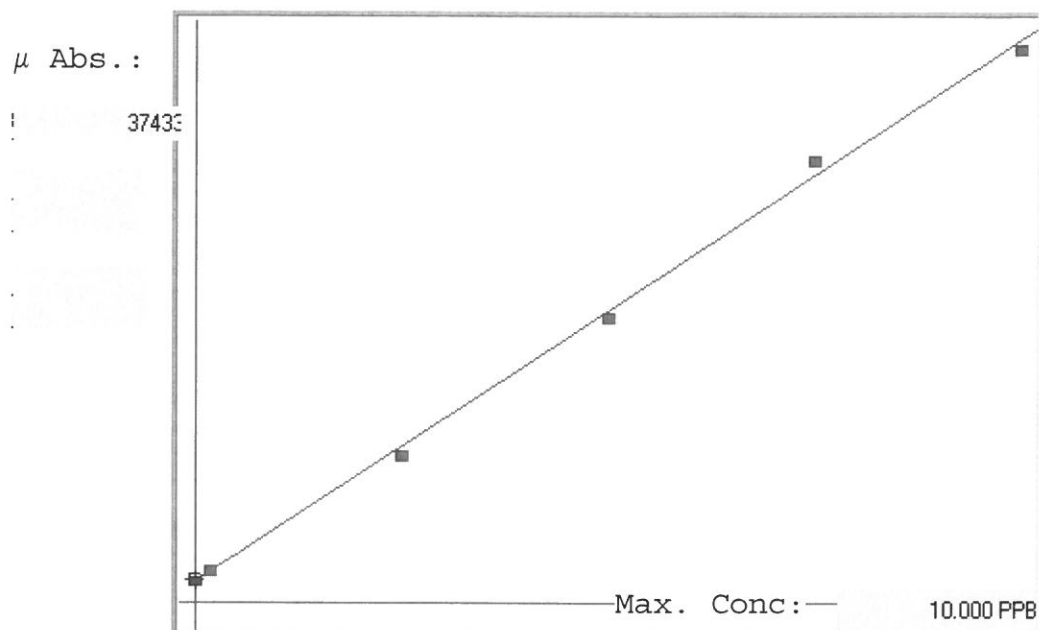

A= 0.0000e+000

B= 2.7301e-004

C= -3.7424e-001

Rho= 0.9990950

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.057	0.057	1578	0.000	1578				
0.2	0.200	0.242	0.042	2257	0.0 %	2257				
2.5	2.500	2.353	-0.147	9991	0.0 %	9991				
5.0	5.000	4.905	-0.095	19339	0.0 %	19339				
7.5	7.500	7.797	0.297	29932	0.0 %	29932				
10.0	10.000	9.845	-0.155	37433	0.0 %	37433				

LB108531 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Apr 2020 08:57:50

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1578	-	0.0000	7470A	PPB	01 Apr 2020 09:25:57	S	Std
0.2 - 1	50.2	2257	-	0.2000	7470A	PPB	01 Apr 2020 09:28:05	S	Std
2.5 - 1	52.5	9991	-	2.5000	7470A	PPB	01 Apr 2020 09:30:12	S	Std
5.0 - 1	55	19339	-	5.0000	7470A	PPB	01 Apr 2020 09:32:20	S	Std
7.5 - 1	57.5	29932	-	7.5000	7470A	PPB	01 Apr 2020 09:34:27	S	Std
10.0 - 1	59	37433	-	10.0000	7470A	PPB	01 Apr 2020 09:39:10	S	Std
ICV84 - 1	ICV84	16411	4.1061	-	7470A	PPB	01 Apr 2020 09:48:23	U	SMPL
ICB84 - 1	ICB84	1294	-0.0210	-	7470A	PPB	01 Apr 2020 09:50:29	U	SMPL
CCV30 - 1	CCV30	19716	5.0084	-	7470A	PPB	01 Apr 2020 09:52:35	U	SMPL
CCB30 - 1	CCB30	1270	-0.0275	-	7470A	PPB	01 Apr 2020 09:54:41	U	SMPL
CRA - 1	CRA	2201	0.2267	-	7470A	PPB	01 Apr 2020 09:59:22	U	SMPL
HighStd - 1	HighStd	38288	10.0787	-	7470A	PPB	01 Apr 2020 10:01:28	U	SMPL
ChkStd - 1	ChkStd	28028	7.2776	-	7470A	PPB	01 Apr 2020 10:03:34	U	SMPL
PB127923BL - 1	PBW	1405	0.0093	-	7470A	PPB	01 Apr 2020 10:05:42	U	SMPL
PB127923BS - 1	LCSW	16484	4.1260	-	7470A	PPB	01 Apr 2020 10:07:50	U	SMPL
L1752-08 - 1	HD-02-033020	1565	0.0530	-	7470A	PPB	01 Apr 2020 10:09:57	U	SMPL
L1752-08DUP - 1	HD-02-033020DUP	1622	0.0686	-	7470A	PPB	01 Apr 2020 10:12:04	U	SMPL
L1752-08MS - 1	HD-02-033020MS	15157	3.7637	-	7470A	PPB	01 Apr 2020 10:14:11	U	SMPL
L1752-08MSD - 1	HD-02-033020MSD	15179	3.7697	-	7470A	PPB	01 Apr 2020 10:16:19	U	SMPL
L1758-06 - 1	PL-03-033020	1616	0.0669	-	7470A	PPB	01 Apr 2020 10:18:26	U	SMPL
CCV31 - 1	CCV31	20227	5.1479	-	7470A	PPB	01 Apr 2020 10:20:32	U	SMPL
CCB31 - 1	CCB31	1273	-0.0267	-	7470A	PPB	01 Apr 2020 10:22:38	U	SMPL
L1759-20 - 1	OR-03-033020	1598	0.0620	-	7470A	PPB	01 Apr 2020 10:24:45	U	SMPL
L1762-25 - 1	TR-04-032720	1336	-0.0095	-	7470A	PPB	01 Apr 2020 10:26:51	U	SMPL
L2070-01 - 1	BUSH-WASH	819	-0.1506	-	7470A	PPB	01 Apr 2020 10:28:57	U	SMPL
L2070-02 - 1	RECLAIM-SYSTEM-SLUDGE-PIT	241	-0.3084	-	7470A	PPB	01 Apr 2020 10:31:04	U	SMPL
L2070-03 - 1	CHASSIS-WASH	1799	0.1169	-	7470A	PPB	01 Apr 2020 10:33:10	U	SMPL
L2070-04 - 1	OIL-WATER-SEPERATOR-SLUDGE-PIT	1998	0.1712	-	7470A	PPB	01 Apr 2020 10:35:17	U	SMPL
L2071-02 - 1	INTERIOR-WALL	1615	0.0667	-	7470A	PPB	01 Apr 2020 10:37:24	U	SMPL
L2071-04 - 1	EXTERIOR-WALL	1656	0.0779	-	7470A	PPB	01 Apr 2020 10:39:32	U	SMPL
L2072-01 - 1	MECHANIC-BUS-LIFT	1711	0.0929	-	7470A	PPB	01 Apr 2020 10:41:39	U	SMPL
L2072-02 - 1	BUS-WASH	2175	0.2196	-	7470A	PPB	01 Apr 2020 10:43:45	U	SMPL
CCV32 - 1	CCV32	19661	4.9934	-	7470A	PPB	01 Apr 2020 10:45:51	U	SMPL
CCB32 - 1	CCB32	1373	0.0006	-	7470A	PPB	01 Apr 2020 10:47:58	U	SMPL
L1752-08LX5 - 1		1606	0.0642	-	7470A	PPB	01 Apr 2020 10:50:05	U	SMPL
L1752-08A - 1		15788	3.9360	-	7470A	PPB	01 Apr 2020 10:52:11	U	SMPL
PB127923TB - 1	PB127896TB	1720	0.0953	-	7470A	PPB	01 Apr 2020 10:54:16	U	SMPL
CCV33 - 1	CCV33	20010	5.0886	-	7470A	PPB	01 Apr 2020 10:56:23	U	SMPL
CCB33 - 1	CCB33	1333	-0.0103	-	7470A	PPB	01 Apr 2020 10:58:30	U	SMPL