


L3108604

7470A

INSTRUMENT ID: CV1

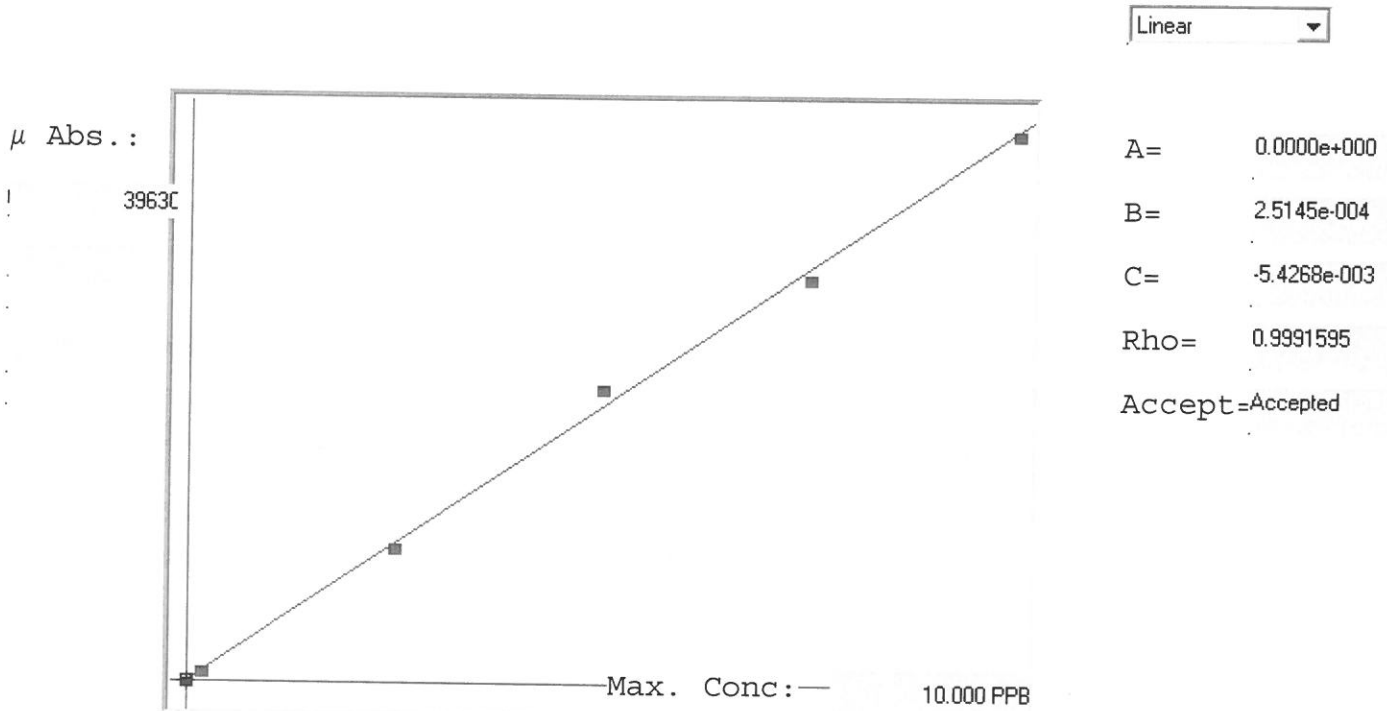

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.018	-0.018	-49	0.000	-49				
0.2	0.200	0.168	-0.032	690	0.0 %	690				
2.5	2.500	2.419	-0.081	9641	0.0 %	9641				
5.0	5.000	5.323	0.323	21192	0.0 %	21192				
7.5	7.500	7.348	-0.152	29243	0.0 %	29243				
10.0	10.000	9.960	-0.040	39630	0.0 %	39630				

LB108604 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Apr 2020 16:01:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-49	-	0.0000	7470A	PPB	06 Apr 2020 16:04:41	S	Std
0.2 - 1	50.2	690	-	0.2000	7470A	PPB	06 Apr 2020 16:06:48	S	Std
2.5 - 1	52.5	9641	-	2.5000	7470A	PPB	06 Apr 2020 16:08:56	S	Std
5.0 - 1	55	21192	-	5.0000	7470A	PPB	06 Apr 2020 16:11:03	S	Std
7.5 - 1	57.5	29243	-	7.5000	7470A	PPB	06 Apr 2020 16:13:10	S	Std
10.0 - 1	51.5	39630	-	10.0000	7470A	PPB	06 Apr 2020 16:15:46	S	Std
ICV86 - 1	ICV86	15822	3.9731	-	7470A	PPB	06 Apr 2020 16:20:44	U	SMPL
ICB86 - 1	ICB86	-10	-0.0079	-	7470A	PPB	06 Apr 2020 16:22:50	U	SMPL
CCV42 - 1	CCV42	21614	5.4295	-	7470A	PPB	06 Apr 2020 16:24:55	U	SMPL
CCB42 - 1	CCB42	-15	-0.0092	-	7470A	PPB	06 Apr 2020 16:27:01	U	SMPL
CRA - 1	CRA	687	0.1673	-	7470A	PPB	06 Apr 2020 16:29:07	U	SMPL
HighStd - 1	HighStd	39968	10.0446	-	7470A	PPB	06 Apr 2020 16:31:12	U	SMPL
ChkStd - 1	ChkStd	25117	6.3103	-	7470A	PPB	06 Apr 2020 16:33:18	U	SMPL
PB128034BL - 1	PBW	54	0.0082	-	7470A	PPB	06 Apr 2020 16:35:26	U	SMPL
PB128034BS - 1	LCSW	15731	3.9502	-	7470A	PPB	06 Apr 2020 16:37:34	U	SMPL
L2097-12 - 1	40772	14	-0.0019	-	7470A	PPB	06 Apr 2020 16:39:41	U	SMPL
L2097-13 - 1	317205	6017	1.5076	-	7470A	PPB	06 Apr 2020 16:41:48	U	SMPL
L2097-14 - 1	40789	3094	0.7726	-	7470A	PPB	06 Apr 2020 16:43:55	U	SMPL
L2097-15 - 1	40788	125	0.0260	-	7470A	PPB	06 Apr 2020 16:48:46	U	SMPL
L2097-16 - 1	40851	873	0.2141	-	7470A	PPB	06 Apr 2020 16:50:51	U	SMPL
CCV43 - 1	CCV43	21560	5.4159	-	7470A	PPB	06 Apr 2020 16:52:57	U	SMPL
CCB43 - 1	CCB43	163	0.0356	-	7470A	PPB	06 Apr 2020 16:55:03	U	SMPL
L2097-18 - 1	COMP-1	107	0.0215	-	7470A	PPB	06 Apr 2020 16:57:09	U	SMPL
L2097-19 - 1	COMP-2	55	0.0084	-	7470A	PPB	06 Apr 2020 16:59:15	U	SMPL
L2099-01 - 1	239-GW-02-12	1771	0.4399	-	7470A	PPB	06 Apr 2020 17:01:21	U	SMPL
L2101-04 - 1	239-WC-L-01	134	0.0283	-	7470A	PPB	06 Apr 2020 17:03:27	U	SMPL
L2126-01 - 1	2-5-1	65	0.0109	-	7470A	PPB	06 Apr 2020 17:05:34	U	SMPL
L2126-02 - 1	2-4-1	380	0.0901	-	7470A	PPB	06 Apr 2020 17:07:41	U	SMPL
L2143-01 - 1	FORMER-OLDEN-AVE-SUB	112	0.0227	-	7470A	PPB	06 Apr 2020 17:09:48	U	SMPL
L2143-01DUP - 1	FORMER-OLDEN-AVE-SUBDUP	116	0.0237	-	7470A	PPB	06 Apr 2020 17:11:56	U	SMPL
L2143-01MS - 1	FORMER-OLDEN-AVE-SUBMS	13536	3.3982	-	7470A	PPB	06 Apr 2020 17:14:04	U	SMPL
L2143-01MSD - 1	FORMER-OLDEN-AVE-SUBMSD	14826	3.7226	-	7470A	PPB	06 Apr 2020 17:16:10	U	SMPL
CCV44 - 1	CCV44	21631	5.4338	-	7470A	PPB	06 Apr 2020 17:18:16	U	SMPL
CCB44 - 1	CCB44	162	0.0353	-	7470A	PPB	06 Apr 2020 17:20:23	U	SMPL
L2152-02 - 1	40734	1540	0.3818	-	7470A	PPB	06 Apr 2020 17:22:29	U	SMPL
L2152-03 - 1	40656	583	0.1412	-	7470A	PPB	06 Apr 2020 17:24:35	U	SMPL
PB128040BL - 1	PBW	135	0.0285	-	7470A	PPB	06 Apr 2020 17:26:41	U	SMPL
PB128040BS - 1	LCSW	15626	3.9238	-	7470A	PPB	06 Apr 2020 17:28:47	U	SMPL
L2110-04 - 1	AU-05-040220	25	0.0009	-	7470A	PPB	06 Apr 2020 17:30:54	U	SMPL
L2112-06 - 1	HR-06-040220	63	0.0104	-	7470A	PPB	06 Apr 2020 17:33:01	U	SMPL
L2112-06DUP - 1	HR-06-040220DUP	52	0.0076	-	7470A	PPB	06 Apr 2020 17:35:09	U	SMPL
L2112-06MS - 1	HR-06-040220MS	16378	4.1129	-	7470A	PPB	06 Apr 2020 17:37:16	U	SMPL
L2112-06MSD - 1	HR-06-040220MSD	17199	4.3193	-	7470A	PPB	06 Apr 2020 17:39:24	U	SMPL
L2145-01 - 1	04-02-A	2	-0.0049	-	7470A	PPB	06 Apr 2020 17:41:30	U	SMPL
CCV45 - 1	CCV45	20961	5.2653	-	7470A	PPB	06 Apr 2020 17:43:36	U	SMPL
CCB45 - 1	CCB45	-29	-0.0127	-	7470A	PPB	06 Apr 2020 17:45:43	U	SMPL
L2145-02 - 1	04-02-B	-87	-0.0273	-	7470A	PPB	06 Apr 2020 17:47:49	U	SMPL
L2145-03 - 1	04-02-C	-73	-0.0238	-	7470A	PPB	06 Apr 2020 17:49:55	U	SMPL
L2145-04 - 1	04-02-D	-61	-0.0208	-	7470A	PPB	06 Apr 2020 17:52:01	U	SMPL
L2145-05 - 1	04-02-E	-59	-0.0203	-	7470A	PPB	06 Apr 2020 17:54:08	U	SMPL
L2152-01 - 1	40732-40733	-72	-0.0235	-	7470A	PPB	06 Apr 2020 17:56:14	U	SMPL
L2161-01 - 1	CHASSIE-WASH	9	-0.0032	-	7470A	PPB	06 Apr 2020 17:58:21	U	SMPL
L2161-02 - 1	RECLAIM-SYSTEM-SEDIMENT-PIT	166	0.0363	-	7470A	PPB	06 Apr 2020 18:00:28	U	SMPL
L2162-13 - 1	TP-50-COMP	-88	-0.0276	-	7470A	PPB	06 Apr 2020 18:02:36	U	SMPL
L2164-03 - 1	ROLL-OFF-COMP	-73	-0.0238	-	7470A	PPB	06 Apr 2020 18:04:43	U	SMPL
L2166-06 - 1	TP-47-COMP	-78	-0.0250	-	7470A	PPB	06 Apr 2020 18:06:49	U	SMPL
CCV46 - 1	CCV46	21077	5.2944	-	7470A	PPB	06 Apr 2020 18:08:56	U	SMPL
CCB46 - 1	CCB46	-27	-0.0122	-	7470A	PPB	06 Apr 2020 18:11:02	U	SMPL
L2166-13 - 1	TP-52-46-COMP	91	0.0175	-	7470A	PPB	06 Apr 2020 18:13:08	U	SMPL
L2166-20 - 1	TP-45-COMP	-71	-0.0233	-	7470A	PPB	06 Apr 2020 18:15:14	U	SMPL
L2143-01LX5 - 1		-162	-0.0462	-	7470A	PPB	06 Apr 2020 18:17:21	U	SMPL
L2143-01A - 1		13298	3.3384	-	7470A	PPB	06 Apr 2020 18:19:27	U	SMPL
L2112-06LX5 - 1		-37	-0.0147	-	7470A	PPB	06 Apr 2020 18:21:34	U	SMPL
L2112-06A - 1		16276	4.0872	-	7470A	PPB	06 Apr 2020 18:23:41	U	SMPL
PB128040TB - 1	PB28012TB	-115	-0.0343	-	7470A	PPB	06 Apr 2020 18:25:48	U	SMPL
CCV47 - 1	CCV47	20928	5.2570	-	7470A	PPB	06 Apr 2020 18:27:55	U	SMPL
CCB47 - 1	CCB47	-18	-0.0100	-	7470A	PPB	06 Apr 2020 18:30:03	U	SMPL