

LB108673


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

41099

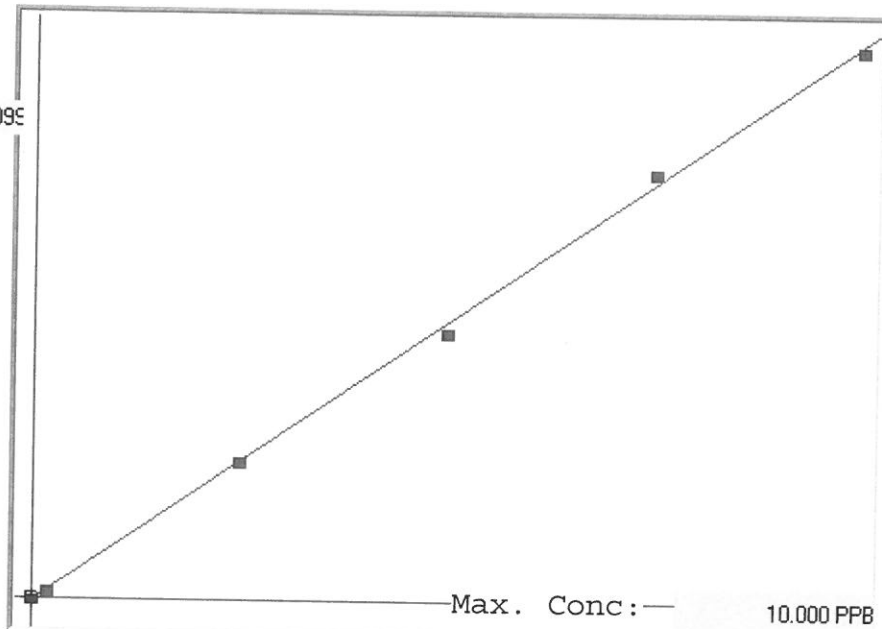

A= 0.0000e+000

B= 2.4055e-004

C= 3.2729e-002

Rho= 0.9994752

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.055	0.055	91	0.000	91				
0.2	0.200	0.178	-0.022	603	0.0 %	603				
2.5	2.500	2.516	0.016	10322	0.0 %	10322				
5.0	5.000	4.823	-0.177	19914	0.0 %	19914				
7.5	7.500	7.710	0.210	31916	0.0 %	31916				
10.0	10.000	9.919	-0.081	41099	0.0 %	41099				

LB108673 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Apr 2020 10:05:17

Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	91	-	0.0007470A		PPB	13 Apr 2020 10:14:08	S	Std
0.2 - 1	50.2	603	-	0.20007470A		PPB	13 Apr 2020 10:16:15	S	Std
2.5 - 1	52.5	10322	-	2.50007470A		PPB	13 Apr 2020 10:18:22	S	Std
5.0 - 1	55	19914	-	5.00007470A		PPB	13 Apr 2020 10:20:30	S	Std
7.5 - 1	57.5	31916	-	7.50007470A		PPB	13 Apr 2020 10:22:37	S	Std
10.0 - 1	510	41099	-	10.00007470A		PPB	13 Apr 2020 10:24:43	S	Std
ICV91 - 1	ICV91	16010	3.8839	-7470A		PPB	13 Apr 2020 10:27:19	U	SMPL
ICB91 - 1	ICB91	-67	0.0166	-7470A		PPB	13 Apr 2020 10:29:25	U	SMPL
CCV84 - 1	CCV84	20088	4.8648	-7470A		PPB	13 Apr 2020 10:31:31	U	SMPL
CCB84 - 1	CCB84	-72	0.0154	-7470A		PPB	13 Apr 2020 10:33:36	U	SMPL
CRA - 1	CRA	596	0.1761	-7470A		PPB	13 Apr 2020 10:35:42	U	SMPL
HighStd - 1	HighStd	41537	10.0243	-7470A		PPB	13 Apr 2020 10:37:47	U	SMPL
ChkStd - 1	ChkStd	29655	7.1661	-7470A		PPB	13 Apr 2020 10:39:53	U	SMPL
PB128162BL - 1	PBW	-151	-0.0036	-7470A		PPB	13 Apr 2020 10:42:01	U	SMPL
PB128162BS - 1	LCSW	14127	3.4309	-7470A		PPB	13 Apr 2020 10:44:09	U	SMPL
L2195-04 - 1	VNJ-223	-39	0.0233	-7470A		PPB	13 Apr 2020 10:46:16	U	SMPL
L2195-04DUP - 1	VNJ-223DUP	24	0.0385	-7470A		PPB	13 Apr 2020 10:48:23	U	SMPL
L2195-04MS - 1	VNJ-223MS	13810	3.3547	-7470A		PPB	13 Apr 2020 10:50:32	U	SMPL
L2195-04MSD - 1	VNJ-223MSD	14268	3.4648	-7470A		PPB	13 Apr 2020 10:52:40	U	SMPL
L2195-08 - 1	VNJ-204	-69	0.0161	-7470A		PPB	13 Apr 2020 10:54:46	U	SMPL
CCV85 - 1	CCV85	20101	4.8680	-7470A		PPB	13 Apr 2020 10:56:52	U	SMPL
CCB85 - 1	CCB85	-43	0.0224	-7470A		PPB	13 Apr 2020 10:58:59	U	SMPL
L2197-01 - 1	CHASSIE-WASH-PIT	29	0.0397	-7470A		PPB	13 Apr 2020 11:01:05	U	SMPL
L2197-02 - 1	FUEL-LANE-SEDIMENT-PIT	66	0.0486	-7470A		PPB	13 Apr 2020 11:03:12	U	SMPL
L2197-03 - 1	BUS-WASH-SEDIMENT-PIT	121	0.0618	-7470A		PPB	13 Apr 2020 11:05:17	U	SMPL
L2197-04 - 1	RECLAIM-SYSTEM-SLUDGE-SEPARATOR	200	0.0808	-7470A		PPB	13 Apr 2020 11:07:23	U	SMPL
L2199-06 - 1	TP-39-38-COMP	27	0.0392	-7470A		PPB	13 Apr 2020 11:09:29	U	SMPL
L2199-13 - 1	TP-37-36-COMP	60	0.0472	-7470A		PPB	13 Apr 2020 11:11:36	U	SMPL
L2201-05 - 1	CG-SUB	69	0.0493	-7470A		PPB	13 Apr 2020 11:13:44	U	SMPL
L2205-08 - 1	JC-02-04082020-A	86	0.0534	-7470A		PPB	13 Apr 2020 11:15:51	U	SMPL
L2205-16 - 1	JC-02-04082020-B	82	0.0525	-7470A		PPB	13 Apr 2020 11:17:59	U	SMPL
L2205-23 - 1	JC-02-04082020-C	55	0.0460	-7470A		PPB	13 Apr 2020 11:20:06	U	SMPL
CCV86 - 1	CCV86	19727	4.7780	-7470A		PPB	13 Apr 2020 11:22:12	U	SMPL
CCB86 - 1	CCB86	-20	0.0279	-7470A		PPB	13 Apr 2020 11:24:18	U	SMPL
PB128163BL - 1	PBW	23	0.0383	-7470A		PPB	13 Apr 2020 11:26:25	U	SMPL
PB128163BS - 1	LCSW	15165	3.6806	-7470A		PPB	13 Apr 2020 11:28:30	U	SMPL
L2215-03 - 1	TP-9	-36	0.0241	-7470A		PPB	13 Apr 2020 11:30:36	U	SMPL
L2215-03DUP - 1	TP-9DUP	29	0.0397	-7470A		PPB	13 Apr 2020 11:32:43	U	SMPL
L2215-03MS - 1	TP-9MS	13734	3.3364	-7470A		PPB	13 Apr 2020 11:34:49	U	SMPL
L2215-03MSD - 1	TP-9MSD	14766	3.5846	-7470A		PPB	13 Apr 2020 11:36:57	U	SMPL
L2215-06 - 1	TP-10	-48	0.0212	-7470A		PPB	13 Apr 2020 11:39:04	U	SMPL
L2215-09 - 1	TP-8	24	0.0385	-7470A		PPB	13 Apr 2020 11:41:11	U	SMPL
L2215-12 - 1	TP-6	28	0.0395	-7470A		PPB	13 Apr 2020 11:43:19	U	SMPL
L2215-15 - 1	TP-4	49	0.0445	-7470A		PPB	13 Apr 2020 11:45:26	U	SMPL
CCV87 - 1	CCV87	20504	4.9649	-7470A		PPB	13 Apr 2020 11:47:32	U	SMPL
CCB87 - 1	CCB87	-23	0.0272	-7470A		PPB	13 Apr 2020 11:49:38	U	SMPL
L2215-18 - 1	TP-3	36	0.0414	-7470A		PPB	13 Apr 2020 11:51:44	U	SMPL
L2215-21 - 1	TP-5	32	0.0404	-7470A		PPB	13 Apr 2020 11:53:51	U	SMPL
L2215-24 - 1	TP-7	31	0.0402	-7470A		PPB	13 Apr 2020 11:55:57	U	SMPL
L2215-27 - 1	TP-1	48	0.0443	-7470A		PPB	13 Apr 2020 11:58:03	U	SMPL
L2215-30 - 1	TP-2	39	0.0421	-7470A		PPB	13 Apr 2020 12:00:10	U	SMPL
L2162-06 - 1	TP-54-53-COMP	57	0.0464	-7470A		PPB	13 Apr 2020 12:02:17	U	SMPL
L2195-04LX5 - 1		31	0.0402	-7470A		PPB	13 Apr 2020 12:04:24	U	SMPL
L2195-04A - 1		16294	3.9522	-7470A		PPB	13 Apr 2020 12:06:32	U	SMPL
L2215-03LX5 - 1		-44	0.0221	-7470A		PPB	13 Apr 2020 12:08:39	U	SMPL
L2215-03A - 1		16389	3.9750	-7470A		PPB	13 Apr 2020 12:10:46	U	SMPL
CCV88 - 1	CCV88	20171	4.8848	-7470A		PPB	13 Apr 2020 12:12:52	U	SMPL
CCB88 - 1	CCB88	-37	0.0238	-7470A		PPB	13 Apr 2020 12:14:58	U	SMPL
PB128162TB - 1	PB128104TB	124	0.0626	-7470A		PPB	13 Apr 2020 12:17:05	U	SMPL
PB128163TB - 1	PB128128TB	70	0.0496	-7470A		PPB	13 Apr 2020 12:19:11	U	SMPL
CCV89 - 1	CCV89	19995	4.8425	-7470A		PPB	13 Apr 2020 12:21:17	U	SMPL
CCB89 - 1	CCB89	-30	0.0255	-7470A		PPB	13 Apr 2020 12:23:23	U	SMPL