


LB 108716

INSTRUMENT ID# CV1

245.1

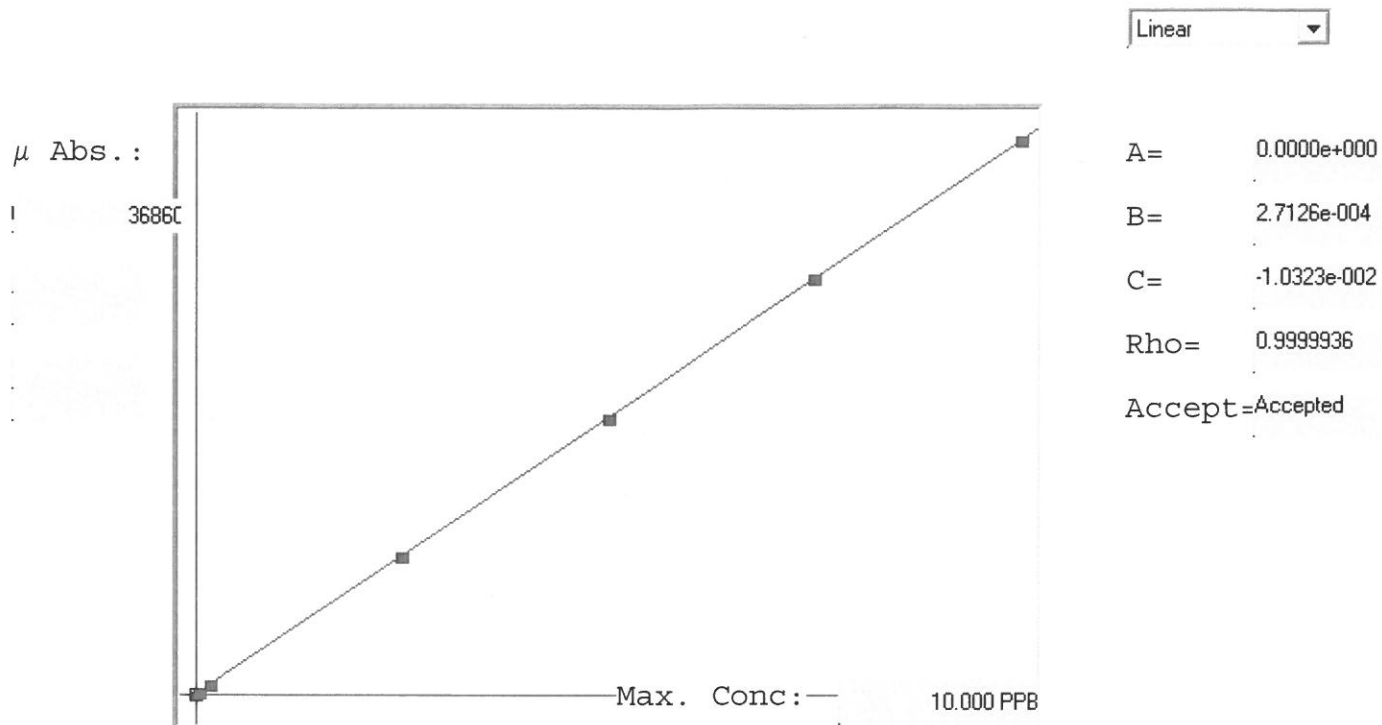

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.004	0.004	54	0.000	54				
0.05	0.050	0.050	0.000	223	0.0 %	223				
0.2	0.200	0.189	-0.011	733	0.0 %	733				
2.5	2.500	2.513	0.013	9301	0.0 %	9301				
5.0	5.000	4.983	-0.017	18410	0.0 %	18410				
7.5	7.500	7.523	0.023	27771	0.0 %	27771				
10.0	10.000	9.988	-0.012	36860	0.0 %	36860				

LB108716 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 15 Apr 2020 09:51:36

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	54	-	0.0000	245.1	PPB	15 Apr 2020 09:53:04	S	Std
0.05 - 1	50.05	223	-	0.0500	245.1	PPB	15 Apr 2020 09:55:21	S	Std
0.2 - 1	50.2	733	-	0.2000	245.1	PPB	15 Apr 2020 09:57:38	S	Std
2.5 - 1	52.5	9301	-	2.5000	245.1	PPB	15 Apr 2020 09:59:55	S	Std
5.0 - 1	55	18410	-	5.0000	245.1	PPB	15 Apr 2020 10:02:11	S	Std
7.5 - 1	57.5	27771	-	7.5000	245.1	PPB	15 Apr 2020 10:04:26	S	Std
10.0 - 1	510	36860	-	10.0000	245.1	PPB	15 Apr 2020 10:06:43	S	Std
ICV96 - 1	ICV96	15336	4.1497	-245.1		PPB	15 Apr 2020 10:12:54	U	SMPL
ICB96 - 1	ICB96	-78	-0.0315	-245.1		PPB	15 Apr 2020 10:15:09	U	SMPL
CCV13 - 1	CCV13	18691	5.0597	-245.1		PPB	15 Apr 2020 10:17:24	U	SMPL
CCB13 - 1	CCB13	-108	-0.0396	-245.1		PPB	15 Apr 2020 10:19:39	U	SMPL
CRA - 1	CRA	187	0.0404	-245.1		PPB	15 Apr 2020 10:21:54	U	SMPL
HighStd - 1	HighStd	37600	10.1889	-245.1		PPB	15 Apr 2020 10:24:09	U	SMPL
ChkStd - 1	ChkStd	26287	7.1202	-245.1		PPB	15 Apr 2020 10:26:24	U	SMPL
PB128223BL - 1	PBW	23	-0.0041	-245.1		PPB	15 Apr 2020 10:31:26	U	SMPL
PB128223BS - 1	LCSW	14742	3.9885	-245.1		PPB	15 Apr 2020 10:33:41	U	SMPL
L2260-01 - 1	OB-722-EB	-91	-0.0350	-245.1		PPB	15 Apr 2020 10:35:57	U	SMPL
L2260-03 - 1	OB-722	45	0.0019	-245.1		PPB	15 Apr 2020 10:38:14	U	SMPL
L2260-04 - 1	OB-722-X	45	0.0019	-245.1		PPB	15 Apr 2020 10:40:30	U	SMPL
L2261-03 - 1	NCQ-632	83	0.0122	-245.1		PPB	15 Apr 2020 10:42:48	U	SMPL
L2261-03DUP - 1	NCQ-632DUP	63	0.0068	-245.1		PPB	15 Apr 2020 10:45:03	U	SMPL
CCV14 - 1	CCV14	18586	5.0312	-245.1		PPB	15 Apr 2020 10:47:18	U	SMPL
CCB14 - 1	CCB14	-105	-0.0388	-245.1		PPB	15 Apr 2020 10:49:33	U	SMPL
L2261-03MS - 1	NCQ-632MS	13684	3.7015	-245.1		PPB	15 Apr 2020 10:51:49	U	SMPL
L2261-03MSD - 1	NCQ-632MSD	14166	3.8323	-245.1		PPB	15 Apr 2020 10:54:03	U	SMPL
L2261-03LX5 - 1		-75	-0.0307	-245.1		PPB	15 Apr 2020 10:56:19	U	SMPL
L2261-03A - 1		17456	4.7247	-245.1		PPB	15 Apr 2020 10:58:34	U	SMPL
CCV15 - 1	CCV15	18402	4.9813	-245.1		PPB	15 Apr 2020 11:00:50	U	SMPL
CCB15 - 1	CCB15	-117	-0.0421	-245.1		PPB	15 Apr 2020 11:03:06	U	SMPL