


LB108784

7471B

INSTRUMENT ID: CV1

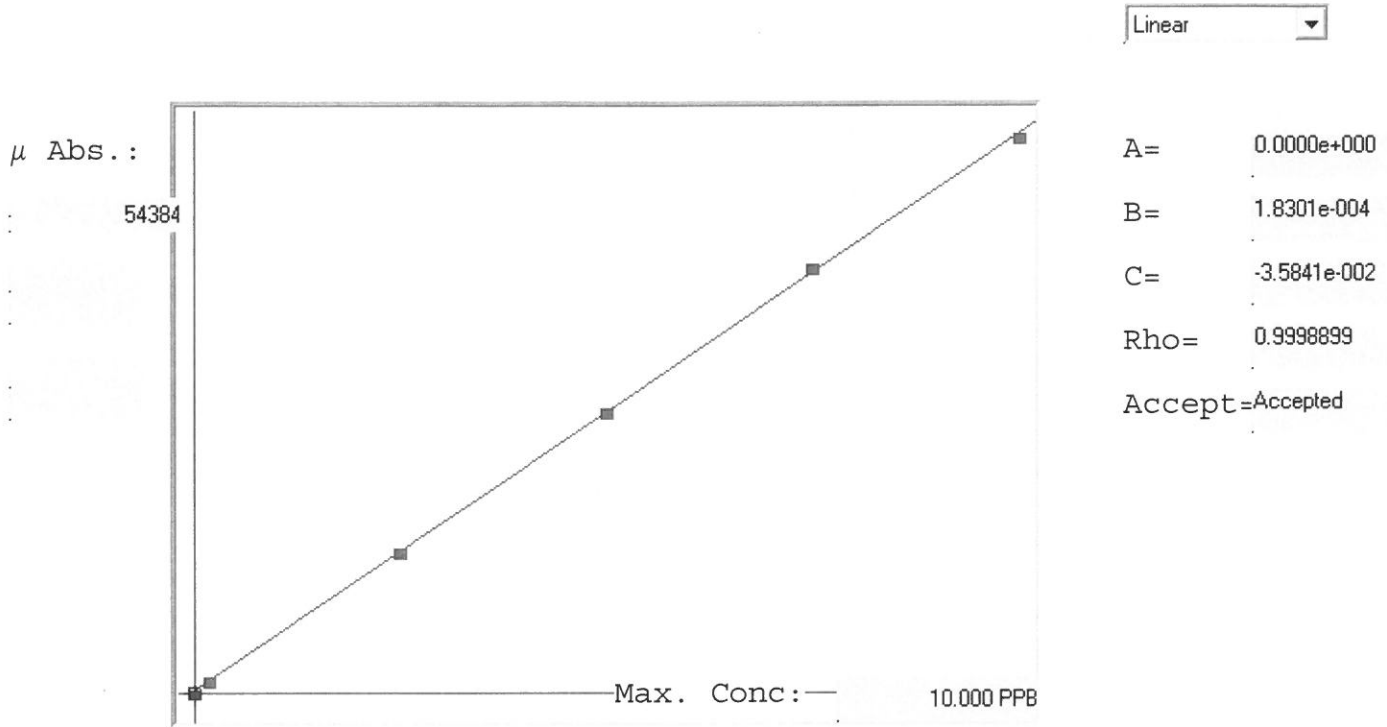

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	162	0.000	162				
0.2	0.200	0.171	-0.029	1131	0.0 %	1131				
2.5	2.500	2.509	0.009	13904	0.0 %	13904				
5.0	5.000	5.009	0.009	27569	0.0 %	27569				
7.5	7.500	7.600	0.100	41725	0.0 %	41725				
10.0	10.000	9.917	-0.083	54384	0.0 %	54384				

LB108764 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 17 Apr 2020 08:26:07			Date	Type	Type
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units			
0.0 - 1	50	162	-	0.0000	7471B	PPB	17 Apr 2020 08:27:28	S	Std
0.2 - 1	50.2	1131	-	0.2000	7471B	PPB	17 Apr 2020 08:34:50	S	Std
2.5 - 1	52.5	13904	-	2.5000	7471B	PPB	17 Apr 2020 08:37:07	S	Std
5.0 - 1	55	27569	-	5.0000	7471B	PPB	17 Apr 2020 08:39:24	S	Std
7.5 - 1	57.5	41725	-	7.5000	7471B	PPB	17 Apr 2020 08:41:40	S	Std
10.0 - 1	57.5	54384	-	10.0000	7471B	PPB	17 Apr 2020 08:43:58	S	Std
ICV02 - 1	ICV02	21677	3.9312	-	7471B	PPB	17 Apr 2020 08:46:43	U	SMPL
ICB02 - 1	ICB02	64	-0.0241	-	7471B	PPB	17 Apr 2020 08:48:58	U	SMPL
CCV38 - 1	CCV38	28087	5.1043	-	7471B	PPB	17 Apr 2020 08:51:14	U	SMPL
CCB38 - 1	CCB38	53	-0.0261	-	7471B	PPB	17 Apr 2020 08:53:28	U	SMPL
CRA - 1	CRA	1148	0.1743	-	7471B	PPB	17 Apr 2020 08:55:44	U	SMPL
HighStd - 1	HighStd	55126	10.0526	-	7471B	PPB	17 Apr 2020 08:57:59	U	SMPL
ChkStd - 1	ChkStd	38175	6.9504	-	7471B	PPB	17 Apr 2020 09:00:14	U	SMPL
PB128293BL - 1	PBS	8	-0.0344	-	7471B	PPB	17 Apr 2020 09:02:31	U	SMPL
PB128293BS - 1	LCSS	19814	3.5903	-	7471B	PPB	17 Apr 2020 09:04:49	U	SMPL
L2308-01 - 1	NCC-TOPSOIL	2744	0.4663	-	7471B	PPB	17 Apr 2020 09:07:06	U	SMPL
L2314-01 - 1	WB-2-1	24506	4.4489	-	7471B	PPB	17 Apr 2020 09:09:23	U	SMPL
L2314-02 - 1	WB-2-2	23247	4.2185	-	7471B	PPB	17 Apr 2020 09:11:40	U	SMPL
L2314-03 - 1	WB-3-1	33953	6.1778	-	7471B	PPB	17 Apr 2020 09:13:58	U	SMPL
L2314-04 - 1	WB-3-2	7428	1.3235	-	7471B	PPB	17 Apr 2020 09:16:14	U	SMPL
CCV39 - 1	CCV39	27678	5.0294	-	7471B	PPB	17 Apr 2020 09:18:31	U	SMPL
CCB39 - 1	CCB39	79	-0.0214	-	7471B	PPB	17 Apr 2020 09:20:46	U	SMPL
L2314-05 - 1	WB-4-1	13757	2.4818	-	7471B	PPB	17 Apr 2020 09:23:03	U	SMPL
L2314-05DUP - 1	WB-4-1DUP	13412	2.4186	-	7471B	PPB	17 Apr 2020 09:25:17	U	SMPL
L2314-06 - 1	WB-4-2	12483	2.2486	-	7471B	PPB	17 Apr 2020 09:27:33	U	SMPL
L2314-07 - 1	WB-5-1	3879	0.6740	-	7471B	PPB	17 Apr 2020 09:29:48	U	SMPL
L2314-08 - 1	WB-5-2	11219	2.0173	-	7471B	PPB	17 Apr 2020 09:32:04	U	SMPL
L2314-09 - 1	DUP-2020-04-15	5955	1.0540	-	7471B	PPB	17 Apr 2020 09:34:20	U	SMPL
L2314-10 - 1	WB-6-1	19815	3.5904	-	7471B	PPB	17 Apr 2020 09:36:36	U	SMPL
L2314-11 - 1	WB-6-2	7585	1.3523	-	7471B	PPB	17 Apr 2020 09:38:53	U	SMPL
L2314-12 - 1	WB-7-1	1981	0.3267	-	7471B	PPB	17 Apr 2020 09:41:10	U	SMPL
L2314-13 - 1	WB-7-2	24392	4.4281	-	7471B	PPB	17 Apr 2020 09:43:26	U	SMPL
CCV40 - 1	CCV40	28027	5.0933	-	7471B	PPB	17 Apr 2020 09:45:41	U	SMPL
CCB40 - 1	CCB40	56	-0.0256	-	7471B	PPB	17 Apr 2020 09:47:57	U	SMPL
L2314-14 - 1	WB-8-1	17128	3.0987	-	7471B	PPB	17 Apr 2020 09:50:13	U	SMPL
L2314-15 - 1	WB-8-2	22195	4.0260	-	7471B	PPB	17 Apr 2020 09:52:28	U	SMPL
L2314-17 - 1	L2314-05MS	32838	5.9737	-	7471B	PPB	17 Apr 2020 09:54:45	U	SMPL
L2314-18 - 1	L2314-05MSD	37993	6.9171	-	7471B	PPB	17 Apr 2020 09:57:01	U	SMPL
L2323-05 - 1	TP-20-COMP	1344	0.2101	-	7471B	PPB	17 Apr 2020 09:59:18	U	SMPL
L2323-12 - 1	TP-19-COMP	1714	0.2778	-	7471B	PPB	17 Apr 2020 10:01:35	U	SMPL
L2324-01 - 1	WC-1	37236	6.7786	-	7471B	PPB	17 Apr 2020 10:03:52	U	SMPL
L2314-05LX5 - 1		2443	0.4112	-	7471B	PPB	17 Apr 2020 10:06:09	U	SMPL
L2314-05A - 1		35530	6.4664	-	7471B	PPB	17 Apr 2020 10:08:26	U	SMPL
CCV41 - 1	CCV41	28066	5.1004	-	7471B	PPB	17 Apr 2020 10:10:42	U	SMPL
CCB41 - 1	CCB41	73	-0.0225	-	7471B	PPB	17 Apr 2020 10:12:59	U	SMPL