


LB108772

7470A

INSTRUMENT ID: CV1

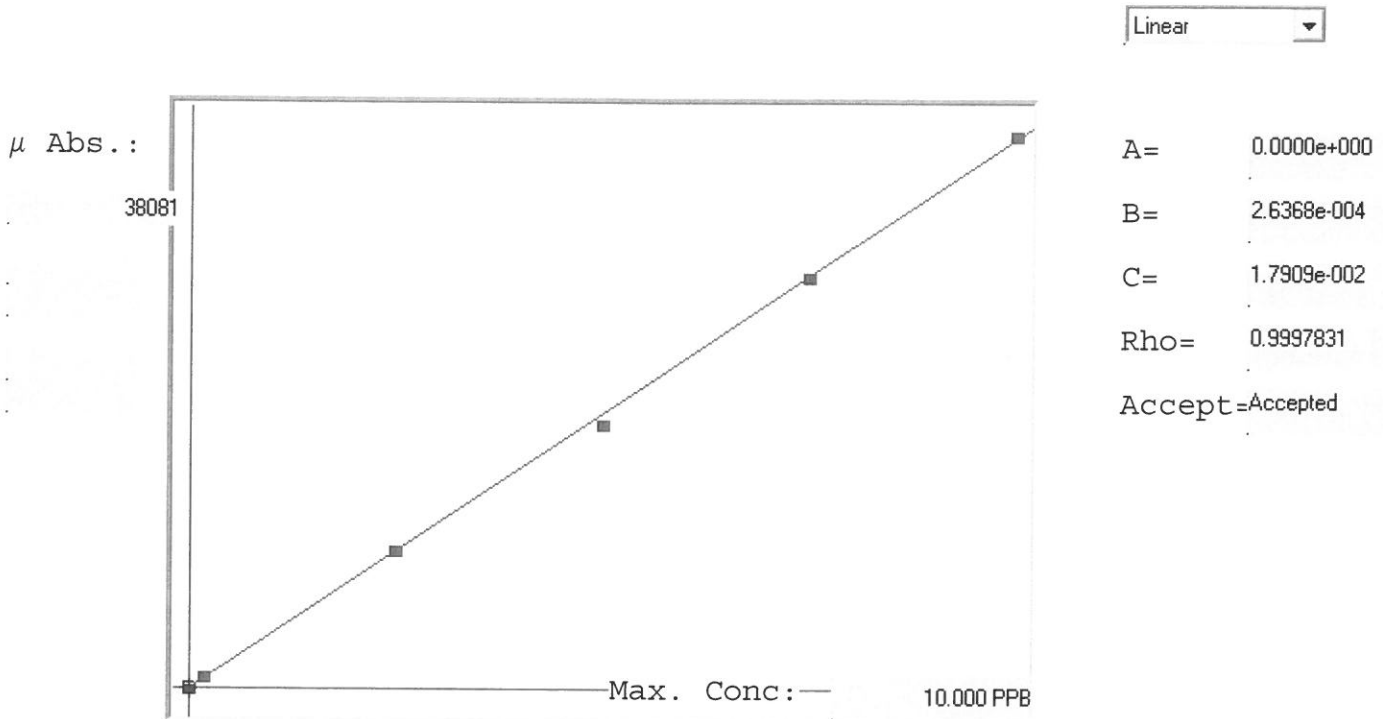

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.029	0.029	41	0.000	41				
0.2	0.200	0.233	0.033	817	0.0 %	817				
2.5	2.500	2.530	0.030	9526	0.0 %	9526				
5.0	5.000	4.830	-0.170	18251	0.0 %	18251				
7.5	7.500	7.519	0.019	28446	0.0 %	28446				
10.0	10.000	10.059	0.059	38081	0.0 %	38081				

LB108772 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Apr 2020 14:34:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	41	-	0.0000	7470A	PPB	17 Apr 2020 14:47:02	S	Std
0.2 - 1	50.2	817	-	0.2000	7470A	PPB	17 Apr 2020 14:49:10	S	Std
2.5 - 1	52.5	9526	-	2.5000	7470A	PPB	17 Apr 2020 14:51:17	S	Std
5.0 - 1	55	18251	-	5.0000	7470A	PPB	17 Apr 2020 14:53:24	S	Std
7.5 - 1	57.5	28446	-	7.5000	7470A	PPB	17 Apr 2020 14:55:32	S	Std
10.0 - 1	57.5	38081	-	10.0000	7470A	PPB	17 Apr 2020 14:57:38	S	Std
ICV03 - 1	ICV03	14641	3.8785	-	7470A	PPB	17 Apr 2020 15:00:11	U	SMPL
ICB03 - 1	ICB03	-50	0.0047	-	7470A	PPB	17 Apr 2020 15:02:17	U	SMPL
CCV44 - 1	CCV44	18565	4.9132	-	7470A	PPB	17 Apr 2020 15:04:22	U	SMPL
CCB44 - 1	CCB44	-51	0.0045	-	7470A	PPB	17 Apr 2020 15:06:28	U	SMPL
CRA - 1	CRA	799	0.2286	-	7470A	PPB	17 Apr 2020 15:08:34	U	SMPL
HighStd - 1	HighStd	37873	10.0044	-	7470A	PPB	17 Apr 2020 15:10:39	U	SMPL
ChkStd - 1	ChkStd	26631	7.0400	-	7470A	PPB	17 Apr 2020 15:12:45	U	SMPL
PB128309BL - 1	PBW	45	0.0298	-	7470A	PPB	17 Apr 2020 15:17:16	U	SMPL
PB128309BS - 1	LCSW	15257	4.0409	-	7470A	PPB	17 Apr 2020 15:19:21	U	SMPL
L2271-15 - 1	BG-3	629	0.1838	-	7470A	PPB	17 Apr 2020 15:21:28	U	SMPL
L2271-16 - 1	BG-1	691	0.2001	-	7470A	PPB	17 Apr 2020 15:23:35	U	SMPL
L2271-17 - 1	BG-2	134	0.0532	-	7470A	PPB	17 Apr 2020 15:25:42	U	SMPL
L2271-18 - 1	BG-4	141	0.0551	-	7470A	PPB	17 Apr 2020 15:27:50	U	SMPL
L2271-18DUP - 1	BG-4DUP	146	0.0564	-	7470A	PPB	17 Apr 2020 15:29:57	U	SMPL
CCV45 - 1	CCV45	18243	4.8283	-	7470A	PPB	17 Apr 2020 15:32:03	U	SMPL
CCB45 - 1	CCB45	-64	0.0010	-	7470A	PPB	17 Apr 2020 15:34:08	U	SMPL
L2271-18MS - 1	BG-4MS	14461	3.8310	-	7470A	PPB	17 Apr 2020 15:36:14	U	SMPL
L2271-18MSD - 1	BG-4MSD	14008	3.7116	-	7470A	PPB	17 Apr 2020 15:38:20	U	SMPL
L2271-21 - 1	BG-8	52	0.0316	-	7470A	PPB	17 Apr 2020 15:40:26	U	SMPL
L2271-22 - 1	DUP-2020-04-13	569	0.1679	-	7470A	PPB	17 Apr 2020 15:42:32	U	SMPL
L2271-23 - 1	BG-7	538	0.1598	-	7470A	PPB	17 Apr 2020 15:44:39	U	SMPL
L2271-24 - 1	BG-6	537	0.1595	-	7470A	PPB	17 Apr 2020 15:46:46	U	SMPL
L2271-25 - 1	BG-5	577	0.1701	-	7470A	PPB	17 Apr 2020 15:48:53	U	SMPL
L2271-26 - 1	BG-9	618	0.1809	-	7470A	PPB	17 Apr 2020 15:52:31	U	SMPL
L2271-27 - 1	BG-10	665	0.1933	-	7470A	PPB	17 Apr 2020 15:54:38	U	SMPL
L2283-09 - 1	PA-2	145	0.0561	-	7470A	PPB	17 Apr 2020 15:56:44	U	SMPL
CCV46 - 1	CCV46	18733	4.9575	-	7470A	PPB	17 Apr 2020 15:58:50	U	SMPL
CCB46 - 1	CCB46	-33	0.0092	-	7470A	PPB	17 Apr 2020 16:00:57	U	SMPL
L2283-10 - 1	PA-3	166	0.0617	-	7470A	PPB	17 Apr 2020 16:03:03	U	SMPL
L2283-11 - 1	PA-1	322	0.1028	-	7470A	PPB	17 Apr 2020 16:05:10	U	SMPL
L2283-12 - 1	PA-5	553	0.1637	-	7470A	PPB	17 Apr 2020 16:07:16	U	SMPL
L2283-13 - 1	PA-4	572	0.1687	-	7470A	PPB	17 Apr 2020 16:09:23	U	SMPL
L2283-14 - 1	WB-1-1	576	0.1698	-	7470A	PPB	17 Apr 2020 16:11:29	U	SMPL
L2283-15 - 1	WB-1-2	166	0.0617	-	7470A	PPB	17 Apr 2020 16:13:36	U	SMPL
PB128310BL - 1	PBW	35	0.0271	-	7470A	PPB	17 Apr 2020 16:18:11	U	SMPL
PB128310BS - 1	LCSW	15296	4.0512	-	7470A	PPB	17 Apr 2020 16:20:18	U	SMPL
L2249-01 - 1	WC-1	612	0.1793	-	7470A	PPB	17 Apr 2020 16:22:26	U	SMPL
L2249-01DUP - 1	WC-1DUP	545	0.1616	-	7470A	PPB	17 Apr 2020 16:27:01	U	SMPL
CCV47 - 1	CCV47	18212	4.8201	-	7470A	PPB	17 Apr 2020 16:35:55	U	SMPL
CCB47 - 1	CCB47	-63	0.0013	-	7470A	PPB	17 Apr 2020 16:38:00	U	SMPL
L2249-01MS - 1	WC-1MS	14216	3.7664	-	7470A	PPB	17 Apr 2020 16:40:06	U	SMPL
L2249-01MSD - 1	WC-1MSD	13625	3.6106	-	7470A	PPB	17 Apr 2020 16:42:13	U	SMPL
L2249-02 - 1	WC-2	512	0.1529	-	7470A	PPB	17 Apr 2020 16:44:19	U	SMPL
L2249-03 - 1	WC-3	568	0.1677	-	7470A	PPB	17 Apr 2020 16:46:25	U	SMPL
L2249-04 - 1	WC-4	616	0.1803	-	7470A	PPB	17 Apr 2020 16:48:31	U	SMPL
L2249-05 - 1	WC-5	439	0.1337	-	7470A	PPB	17 Apr 2020 16:50:38	U	SMPL
L2249-06 - 1	WC-6	166	0.0617	-	7470A	PPB	17 Apr 2020 16:52:45	U	SMPL
L2249-07 - 1	WC-7	746	0.2146	-	7470A	PPB	17 Apr 2020 16:54:53	U	SMPL
PB128311BL - 1	PBW	45	0.0298	-	7470A	PPB	17 Apr 2020 16:57:00	U	SMPL
PB128311BS - 1	LCSW	14844	3.9320	-	7470A	PPB	17 Apr 2020 16:59:07	U	SMPL
CCV48 - 1	CCV48	17606	4.6603	-	7470A	PPB	17 Apr 2020 17:01:13	U	SMPL
CCB48 - 1	CCB48	-43	0.0066	-	7470A	PPB	17 Apr 2020 17:03:19	U	SMPL
L2305-01 - 1	I-OC-1	412	0.1265	-	7470A	PPB	17 Apr 2020 17:12:11	U	SMPL
L2305-01DUP - 1	I-OC-1DUP	338	0.1070	-	7470A	PPB	17 Apr 2020 17:14:17	U	SMPL
L2305-01MS - 1	I-OC-1MS	13270	3.5170	-	7470A	PPB	17 Apr 2020 17:16:24	U	SMPL
L2305-01MSD - 1	I-OC-1MSD	13807	3.6586	-	7470A	PPB	17 Apr 2020 17:18:30	U	SMPL
L2305-05 - 1	I-R-1	972	0.2742	-	7470A	PPB	17 Apr 2020 17:20:37	U	SMPL
L2305-06 - 1	E-R-1	676	0.1962	-	7470A	PPB	17 Apr 2020 17:22:44	U	SMPL
L2314-16 - 1	FB-2020-04-15	111	0.0472	-	7470A	PPB	17 Apr 2020 17:24:51	U	SMPL
CCV49 - 1	CCV49	19419	5.1384	-	7470A	PPB	17 Apr 2020 17:26:59	U	SMPL
CCB49 - 1	CCB49	-47	0.0055	-	7470A	PPB	17 Apr 2020 17:29:06	U	SMPL
L2271-18LX5 - 1		13	0.0213	-	7470A	PPB	17 Apr 2020 17:31:11	U	SMPL
L2271-18A - 1		14742	3.9051	-	7470A	PPB	17 Apr 2020 17:33:18	U	SMPL
L2249-01LX5 - 1		102	0.0448	-	7470A	PPB	17 Apr 2020 17:35:25	U	SMPL
L2249-01A - 1		15133	4.0082	-	7470A	PPB	17 Apr 2020 17:37:32	U	SMPL
L2305-01A - 1		15298	4.0517	-	7470A	PPB	17 Apr 2020 17:41:44	U	SMPL
PB128309TB - 1	PB128278TB	-6	0.0163	-	7470A	PPB	17 Apr 2020 17:43:51	U	SMPL
PB128310TB - 1	PB128297TB	38	0.0279	-	7470A	PPB	17 Apr 2020 17:45:58	U	SMPL
L2305-01LX5 - 1		49	0.0308	-	7470A	PPB	17 Apr 2020 17:58:34	U	SMPL
CCV50 - 1	CCV50	19032	5.0363	-	7470A	PPB	17 Apr 2020 18:00:57	U	SMPL
CCB50 - 1	CCB50	0	0.0179	-	7470A	PPB	17 Apr 2020 18:03:04	U	SMPL