

LB108818

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : OK

Instrument ID : Konelab

4/21/2020 15:35

Test: ^{puke} ~~Total~~ CN *my 1c*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.289	0.0	0.086	
ICB1	0.918	0.0	0.004	
CCV1	245.554	0.0	0.212	
CCB1	0.967	0.0	0.004	
PB128350BL	0.768	0.0	0.003	
L2310-01	0.793	0.0	0.003	
L2310-01DUP	0.781	0.0	0.003	
L2323-06	0.821	0.0	0.003	
L2323-13	0.750	0.0	0.003	
L2327-03	0.705	0.0	0.003	
L2327-06	0.660	0.0	0.003	
L2327-09	0.654	0.0	0.003	
L2327-12	0.712	0.0	0.003	
CCV2	247.055	0.0	0.213	
CCB2	0.822	0.0	0.003	
L2327-18	0.752	0.0	0.003	
L2327-21	0.676	0.0	0.003	
L2327-24	0.494	0.0	0.003	
L2332-03	0.599	0.0	0.003	
L2332-06	0.682	0.0	0.003	
L2339-03	0.586	0.0	0.003	
L2344-03	0.462	0.0	0.003	
L2350-03	0.525	0.0	0.003	
L2350-06	0.625	0.0	0.003	
PB128398BL	0.721	0.0	0.003	
CCV3	246.590	0.0	0.213	
CCB3	0.620	0.0	0.003	
L2123-14	0.806	0.0	0.003	
L2123-14DUP	0.482	0.0	0.003	
L2311-01	0.592	0.0	0.003	
L2331-04	0.561	0.0	0.003	
L2331-08	0.531	0.0	0.003	
L2351-04	0.671	0.0	0.003	
L2351-08	0.390	0.0	0.003	
L2351-12	0.623	0.0	0.003	
L2353-04	-0.006	0.0	0.003	
L2357-04	0.622	0.0	0.003	
CCV4	256.983	0.0	0.222	
CCB4	0.635	0.0	0.003	
L2359-04	0.697	0.0	0.003	
L2359-08	0.801	0.0	0.003	
L2327-15	0.765	0.0	0.003	
CCV5	270.804	0.0	0.233	
CCB5	0.857	0.0	0.003	

N 44
 Mean 31.577
 SD 81.7148
 CV% 258.78

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 21 14:44:58 2020

Tue Apr 21 15:18:19 2020

DA

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	0.2945	µg/l	4/21/2020 11:59:08	
5.OPPBCN	A	REACTIVE CN	P	5.1153	µg/l	4/21/2020 11:59:09	
10PPBCN	A	REACTIVE CN	P	9.6779	µg/l	4/21/2020 11:59:10	
50PPBCN	A	REACTIVE CN	P	50.2682	µg/l	4/21/2020 11:59:11	
100PPBCN	A	REACTIVE CN	P	98.2381	µg/l	4/21/2020 11:59:12	
250PPBCN	A	REACTIVE CN	P	252.1503	µg/l	4/21/2020 11:59:13	
500PPBCN	A	REACTIVE CN	P	499.2557	µg/l	4/21/2020 11:59:14	
ICV1	S	REACTIVE CN	P	97.2894	µg/l	4/21/2020 14:44:59	
ICB1	S	REACTIVE CN	P	0.9178	µg/l	4/21/2020 14:45:00	
CCV1	S	REACTIVE CN	P	245.5536	µg/l	4/21/2020 14:45:03	
CCB1	S	REACTIVE CN	P	0.9669	µg/l	4/21/2020 14:45:05	
PB128350BL	S	REACTIVE CN	P	0.7683	µg/l	4/21/2020 14:45:06	
L2310-01	S	REACTIVE CN	P	0.7929	µg/l	4/21/2020 14:45:07	
L2310-01DUP	S	REACTIVE CN	P	0.7808	µg/l	4/21/2020 14:45:08	
L2323-06	S	REACTIVE CN	P	0.8213	µg/l	4/21/2020 14:52:34	
L2323-13	S	REACTIVE CN	P	0.7504	µg/l	4/21/2020 14:52:35	
L2327-03	S	REACTIVE CN	P	0.7053	µg/l	4/21/2020 14:52:36	
L2327-06	S	REACTIVE CN	P	0.6602	µg/l	4/21/2020 14:52:37	
L2327-09	S	REACTIVE CN	P	0.6544	µg/l	4/21/2020 14:52:38	
L2327-12	S	REACTIVE CN	P	0.7122	µg/l	4/21/2020 14:52:39	
CCV2	S	REACTIVE CN	P	247.0546	µg/l	4/21/2020 14:52:42	
CCB2	S	REACTIVE CN	P	0.8217	µg/l	4/21/2020 14:52:44	
L2327-18	S	REACTIVE CN	P	0.7518	µg/l	4/21/2020 15:00:08	
L2327-21	S	REACTIVE CN	P	0.676	µg/l	4/21/2020 15:00:09	
L2327-24	S	REACTIVE CN	P	0.4939	µg/l	4/21/2020 15:00:10	
L2332-03	S	REACTIVE CN	P	0.5988	µg/l	4/21/2020 15:00:11	
L2332-06	S	REACTIVE CN	P	0.6821	µg/l	4/21/2020 15:00:12	
L2339-03	S	REACTIVE CN	P	0.5856	µg/l	4/21/2020 15:00:13	
L2344-03	S	REACTIVE CN	P	0.4617	µg/l	4/21/2020 15:00:14	
L2350-03	S	REACTIVE CN	P	0.5254	µg/l	4/21/2020 15:00:15	
L2350-06	S	REACTIVE CN	P	0.6246	µg/l	4/21/2020 15:00:16	
PB128398BL	S	REACTIVE CN	P	0.7207	µg/l	4/21/2020 15:00:17	
CCV3	S	REACTIVE CN	P	246.5897	µg/l	4/21/2020 15:00:18	
CCB3	S	REACTIVE CN	P	0.6202	µg/l	4/21/2020 15:07:40	
L2123-14	S	REACTIVE CN	P	0.8059	µg/l	4/21/2020 15:07:41	
L2123-14DUP	S	REACTIVE CN	P	0.4823	µg/l	4/21/2020 15:07:42	
L2311-01	S	REACTIVE CN	P	0.5922	µg/l	4/21/2020 15:07:43	
L2331-04	S	REACTIVE CN	P	0.5613	µg/l	4/21/2020 15:07:44	
L2331-08	S	REACTIVE CN	P	0.5315	µg/l	4/21/2020 15:07:45	
L2351-04	S	REACTIVE CN	P	0.6709	µg/l	4/21/2020 15:07:46	
L2351-08	S	REACTIVE CN	P	0.3896	µg/l	4/21/2020 15:07:47	
L2351-12	S	REACTIVE CN	P	0.6234	µg/l	4/21/2020 15:07:48	

L2353-04	S	REACTIVE CN	P	-0.0061 µg/l	4/21/2020 15:07:49
L2357-04	S	REACTIVE CN	P	0.6218 µg/l	4/21/2020 15:07:50
CCV4	S	REACTIVE CN	P	256.9832 µg/l	4/21/2020 15:12:56
CCB4	S	REACTIVE CN	P	0.6354 µg/l	4/21/2020 15:12:57
L2359-04	S	REACTIVE CN	P	0.697 µg/l	4/21/2020 15:12:58
L2359-08	S	REACTIVE CN	P	0.8007 µg/l	4/21/2020 15:12:59
L2327-15	S	REACTIVE CN	P	0.7653 µg/l	4/21/2020 15:18:17
CCV5	S	REACTIVE CN	P	270.8041 µg/l	4/21/2020 15:18:18
CCB5	S	REACTIVE CN	P	0.857 µg/l	4/21/2020 15:18:19

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : JK

Instrument ID : Konelab

4/21/2020 15:39


Test Residue
~~Total~~ CN

Accepted 4/21/2020 12:09

Factor 1174
Bias 0.003

Coeff. of det. 0.999958

Errors

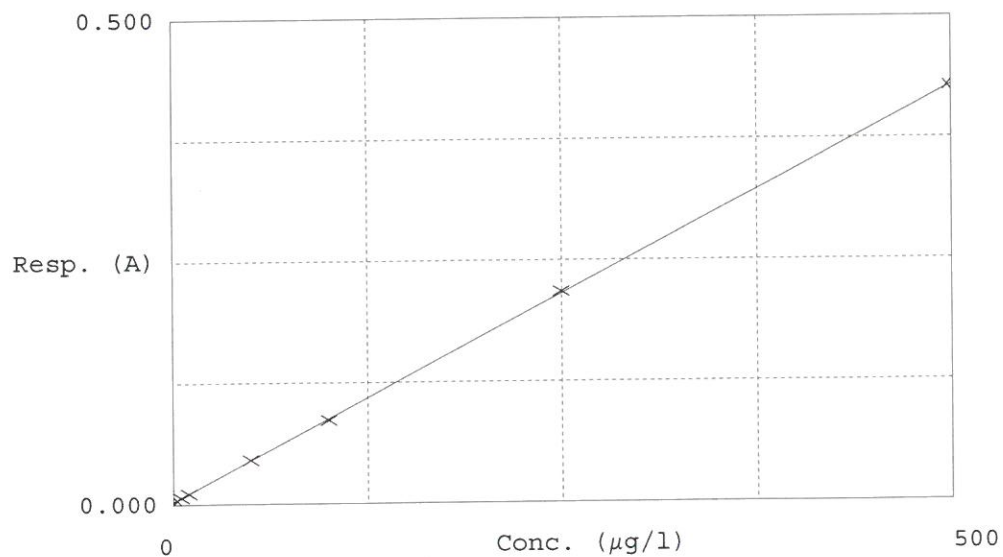

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.2945	0.0000	
2	5.0PPBCN	0.007	5.1153	5.0000	
3	10PPBCN	0.011	9.6779	10.0000	
4	50PPBCN	0.046	50.2682	50.0000	
5	100PPBCN	0.086	98.2381	100.0000	
6	250PPBCN	0.218	252.1503	250.0000	
7	500PPBCN	0.428	499.2557	500.0000	