


LB108844

7471B

INSTRUMENT ID: CY1

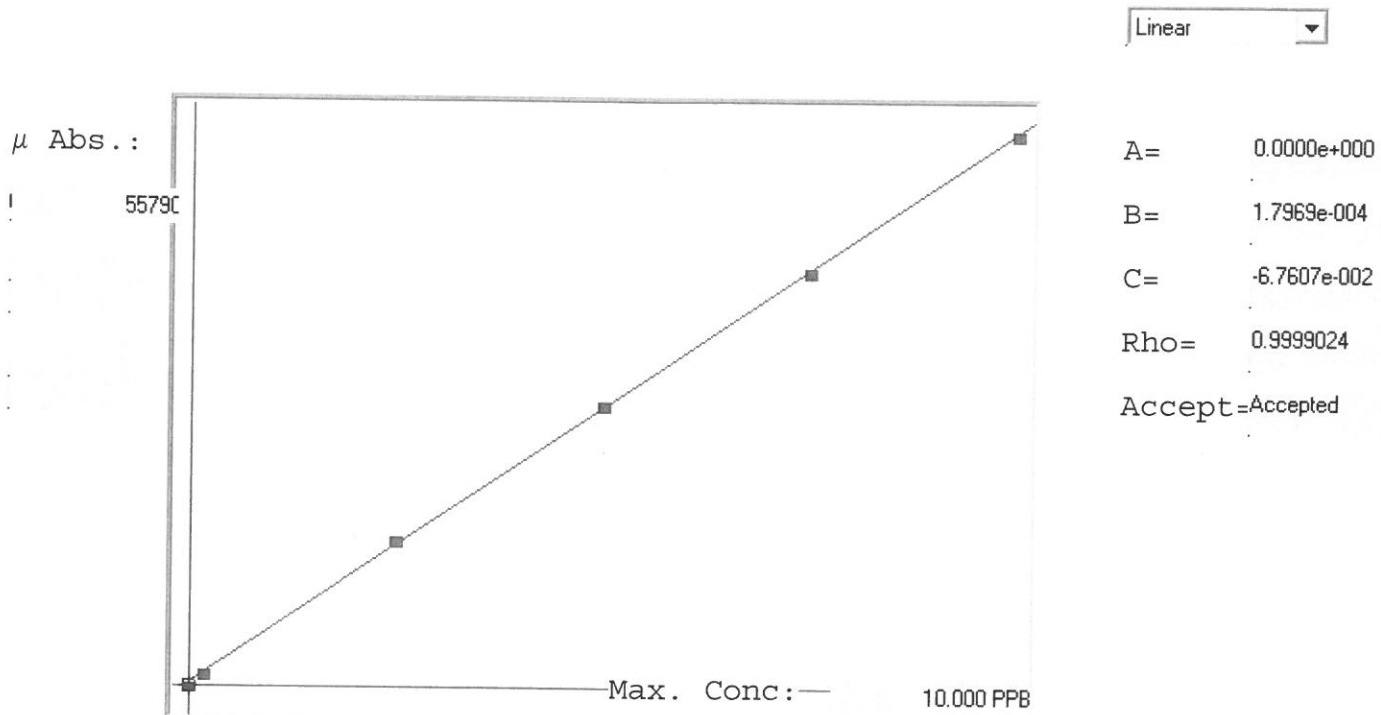

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.047	-0.047	115	0.000	115				
0.2	0.200	0.159	-0.041	1259	0.0 %	1259				
2.5	2.500	2.588	0.088	14780	0.0 %	14780				
5.0	5.000	5.049	0.049	28474	0.0 %	28474				
7.5	7.500	7.494	-0.006	42078	0.0 %	42078				
10.0	10.000	9.958	-0.042	55790	0.0 %	55790				

LB108844 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Apr 2020 10:12:24

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	115	-	0.00007471B	PPB	23 Apr 2020 10:14:45	S	Std
0.2 - 1	50.2	1259	-	0.20007471B	PPB	23 Apr 2020 10:17:01	S	Std
2.5 - 1	52.5	14780	-	2.50007471B	PPB	23 Apr 2020 10:19:18	S	Std
5.0 - 1	55	28474	-	5.00007471B	PPB	23 Apr 2020 10:21:35	S	Std
7.5 - 1	57.5	42078	-	7.50007471B	PPB	23 Apr 2020 10:23:52	S	Std
10.0 - 1	510	55790	-	10.00007471B	PPB	23 Apr 2020 10:26:08	S	Std
ICV11 - 1	ICV11	21512	3.7980	-7471B	PPB	23 Apr 2020 10:29:12	U	SMPL
ICB11 - 1	ICB11	-11	-0.0696	-7471B	PPB	23 Apr 2020 10:31:26	U	SMPL
CCV82 - 1	CCV82	28795	5.1067	-7471B	PPB	23 Apr 2020 10:33:42	U	SMPL
CCB82 - 1	CCB82	-14	-0.0701	-7471B	PPB	23 Apr 2020 10:35:57	U	SMPL
CRA - 1	CRA	1243	0.1558	-7471B	PPB	23 Apr 2020 10:38:12	U	SMPL
HighStd - 1	HighStd	55990	9.9934	-7471B	PPB	23 Apr 2020 10:40:27	U	SMPL
ChkStd - 1	ChkStd	40228	7.1611	-7471B	PPB	23 Apr 2020 10:42:43	U	SMPL
PB128434BL - 1	PBS	-81	-0.0822	-7471B	PPB	23 Apr 2020 10:45:00	U	SMPL
PB128434BS - 1	LCSS	21204	3.7426	-7471B	PPB	23 Apr 2020 10:47:17	U	SMPL
L2117-06 - 1	OK-01-042220	3669	0.5917	-7471B	PPB	23 Apr 2020 10:49:34	U	SMPL
L2120-01 - 1	OR-02-042220	3377	0.5392	-7471B	PPB	23 Apr 2020 10:51:51	U	SMPL
L2360-01 - 1	GREENWALL	2452	0.3730	-7471B	PPB	23 Apr 2020 10:54:08	U	SMPL
L2360-02 - 1	CONCRETE FLOOR	4970	0.8255	-7471B	PPB	23 Apr 2020 10:56:25	U	SMPL
L2360-03 - 1	OUTSIDE WALL	196	-0.0324	-7471B	PPB	23 Apr 2020 10:58:40	U	SMPL
CCV83 - 1	CCV83	28797	5.1070	-7471B	PPB	23 Apr 2020 11:00:55	U	SMPL
CCB83 - 1	CCB83	20	-0.0640	-7471B	PPB	23 Apr 2020 11:03:11	U	SMPL
L2374-02 - 1	WC-1A	3647	0.5877	-7471B	PPB	23 Apr 2020 11:05:27	U	SMPL
L2377-01 - 1	MILL-1	4344	0.7130	-7471B	PPB	23 Apr 2020 11:07:43	U	SMPL
L2378-03 - 1	TP-6-S	6132	1.0343	-7471B	PPB	23 Apr 2020 11:14:45	U	SMPL
L2378-03DUP - 1	TP-6-SDUP	5503	0.9212	-7471B	PPB	23 Apr 2020 11:17:00	U	SMPL
L2378-03MS - 1	TP-6-SMS	25340	4.4858	-7471B	PPB	23 Apr 2020 11:19:16	U	SMPL
L2378-03MSD - 1	TP-6-SMSD	26359	4.6689	-7471B	PPB	23 Apr 2020 11:21:32	U	SMPL
L2378-07 - 1	TP-3-S	21481	3.7924	-7471B	PPB	23 Apr 2020 11:23:49	U	SMPL
L2378-11 - 1	TP-2-S	817	0.0792	-7471B	PPB	23 Apr 2020 11:26:06	U	SMPL
L2381-01 - 1	ETGI-337	1368	0.1782	-7471B	PPB	23 Apr 2020 11:28:23	U	SMPL
L2383-01 - 1	ETGI-355-72-11939	449	0.0131	-7471B	PPB	23 Apr 2020 11:30:39	U	SMPL
CCV84 - 1	CCV84	29086	5.1590	-7471B	PPB	23 Apr 2020 11:32:54	U	SMPL
CCB84 - 1	CCB84	2	-0.0672	-7471B	PPB	23 Apr 2020 11:35:09	U	SMPL
L2383-04 - 1	VNJ-239	5123	0.8530	-7471B	PPB	23 Apr 2020 11:37:25	U	SMPL
L2394-01 - 1	R-1	4464	0.7345	-7471B	PPB	23 Apr 2020 11:39:40	U	SMPL
L2394-03 - 1	B-1	3795	0.6143	-7471B	PPB	23 Apr 2020 11:41:56	U	SMPL
L2394-05 - 1	O-1	1097	0.1295	-7471B	PPB	23 Apr 2020 11:44:11	U	SMPL
L2394-07 - 1	G-1	7348	1.2528	-7471B	PPB	23 Apr 2020 11:46:27	U	SMPL
L2397-05 - 1	TP-1-COMP	2173	0.3229	-7471B	PPB	23 Apr 2020 11:48:43	U	SMPL
L2378-03LX5 - 1		1213	0.1504	-7471B	PPB	23 Apr 2020 11:50:59	U	SMPL
L2378-03A - 1		26963	4.7775	-7471B	PPB	23 Apr 2020 11:53:16	U	SMPL
CCV85 - 1	CCV85	28583	5.0686	-7471B	PPB	23 Apr 2020 12:10:16	U	SMPL
CCB85 - 1	CCB85	40	-0.0604	-7471B	PPB	23 Apr 2020 12:12:31	U	SMPL