


LB10880

245.1

INSTRUMENT ID: CV1

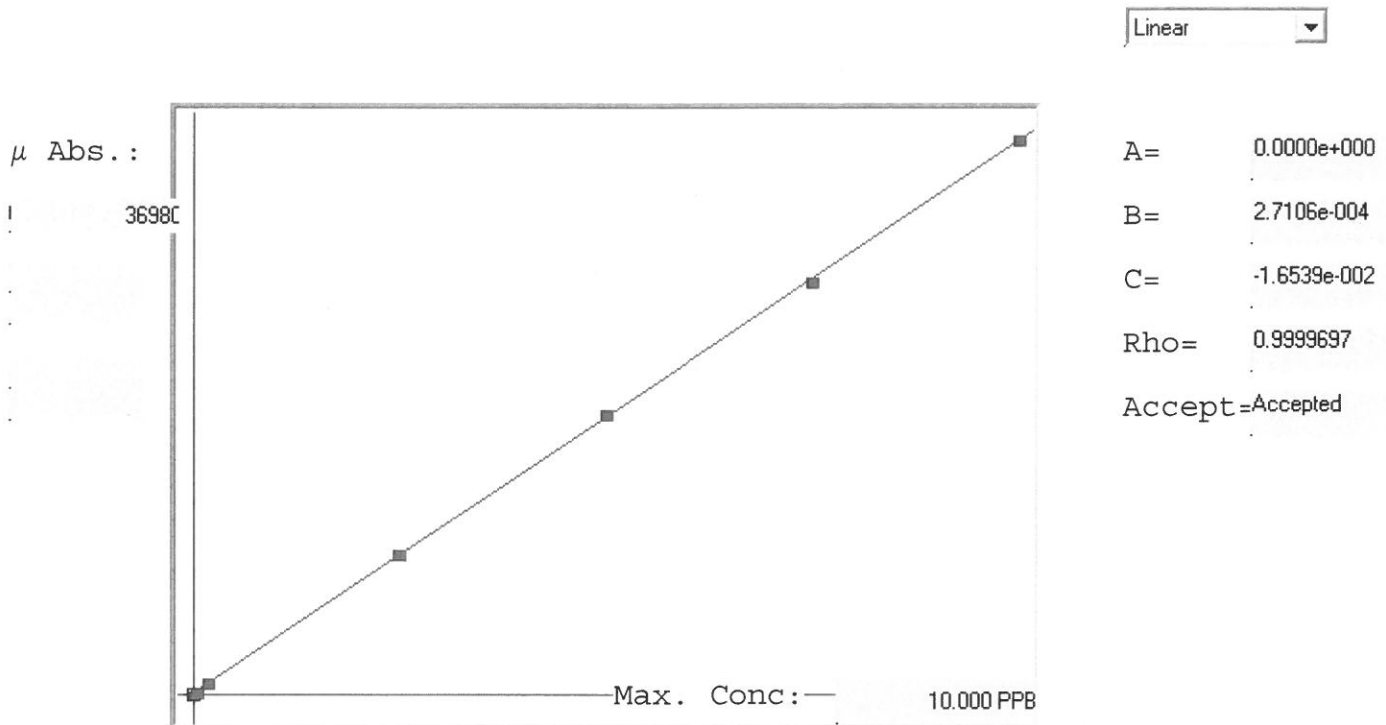

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	17	0.000	17				
0.05	0.050	0.041	-0.009	212	0.0 %	212				
0.2	0.200	0.193	-0.007	773	0.0 %	773				
2.5	2.500	2.521	0.021	9363	0.0 %	9363				
5.0	5.000	5.050	0.050	18692	0.0 %	18692				
7.5	7.500	7.449	-0.051	27544	0.0 %	27544				
10.0	10.000	10.007	0.007	36980	0.0 %	36980				

LB108880 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 27 Apr 2020 11:26:00

Sample ID	Extended ID	μ Abs.	Conc.	Stnd ConcMethod	Units	Date	Type	Type
0.0 - 1	50	17	-	0.0000245.1	PPB	27 Apr 2020 11:29:00	S	Std
0.05 - 1	50.05	212	-	0.0500245.1	PPB	27 Apr 2020 11:31:16	S	Std
0.2 - 1	50.2	773	-	0.2000245.1	PPB	27 Apr 2020 11:33:34	S	Std
2.5 - 1	52.5	9363	-	2.5000245.1	PPB	27 Apr 2020 11:35:50	S	Std
5.0 - 1	55	18692	-	5.0000245.1	PPB	27 Apr 2020 11:38:06	S	Std
7.5 - 1	57.5	27544	-	7.5000245.1	PPB	27 Apr 2020 11:40:21	S	Std
10.0 - 1	57.1	36980	-	10.0000245.1	PPB	27 Apr 2020 11:57:37	S	Std
ICV16 - 1	ICV16	15126	4.0835	-245.1	PPB	27 Apr 2020 12:02:51	U	SMPL
ICB16 - 1	ICB16	-93	-0.0417	-245.1	PPB	27 Apr 2020 12:05:06	U	SMPL
CCV01 - 1	CCV01	18890	5.1037	-245.1	PPB	27 Apr 2020 12:07:21	U	SMPL
CCB01 - 1	CCB01	-111	-0.0466	-245.1	PPB	27 Apr 2020 12:09:35	U	SMPL
CRA - 1	CRA	209	0.0401	-245.1	PPB	27 Apr 2020 12:16:57	U	SMPL
HighStd - 1	HighStd	36153	9.7830	-245.1	PPB	27 Apr 2020 12:19:11	U	SMPL
ChkStd - 1	ChkStd	26534	7.1757	-245.1	PPB	27 Apr 2020 12:21:27	U	SMPL
PB128494BL - 1	PBW	31	-0.0081	-245.1	PPB	27 Apr 2020 12:26:16	U	SMPL
PB128494BS - 1	LCSW	14004	3.7793	-245.1	PPB	27 Apr 2020 12:28:32	U	SMPL
L2182-12 - 1	MDL-WATER-06-QT2-2020	225	0.0444	-245.1	PPB	27 Apr 2020 12:35:55	U	SMPL
L2408-03 - 1	HP-627	107	0.0125	-245.1	PPB	27 Apr 2020 12:38:12	U	SMPL
L2408-03DUP - 1	HP-627DUP	118	0.0154	-245.1	PPB	27 Apr 2020 12:40:28	U	SMPL
L2408-03MS - 1	HP-627MS	13614	3.6736	-245.1	PPB	27 Apr 2020 12:42:46	U	SMPL
L2408-03MSD - 1	HP-627MSD	13528	3.6503	-245.1	PPB	27 Apr 2020 12:47:46	U	SMPL
CCV02 - 1	CCV02	19044	5.1455	-245.1	PPB	27 Apr 2020 12:50:00	U	SMPL
CCB02 - 1	CCB02	-84	-0.0393	-245.1	PPB	27 Apr 2020 12:52:16	U	SMPL
L2408-03LX5 - 1		23	-0.0103	-245.1	PPB	27 Apr 2020 12:54:32	U	SMPL
L2408-03A - 1		14384	3.8823	-245.1	PPB	27 Apr 2020 12:56:47	U	SMPL
CCV03 - 1	CCV03	19383	5.2374	-245.1	PPB	27 Apr 2020 12:59:03	U	SMPL
CCB03 - 1	CCB03	-102	-0.0442	-245.1	PPB	27 Apr 2020 13:01:18	U	SMPL