


LB108991

7471B

INSTRUMENT ID: CV2

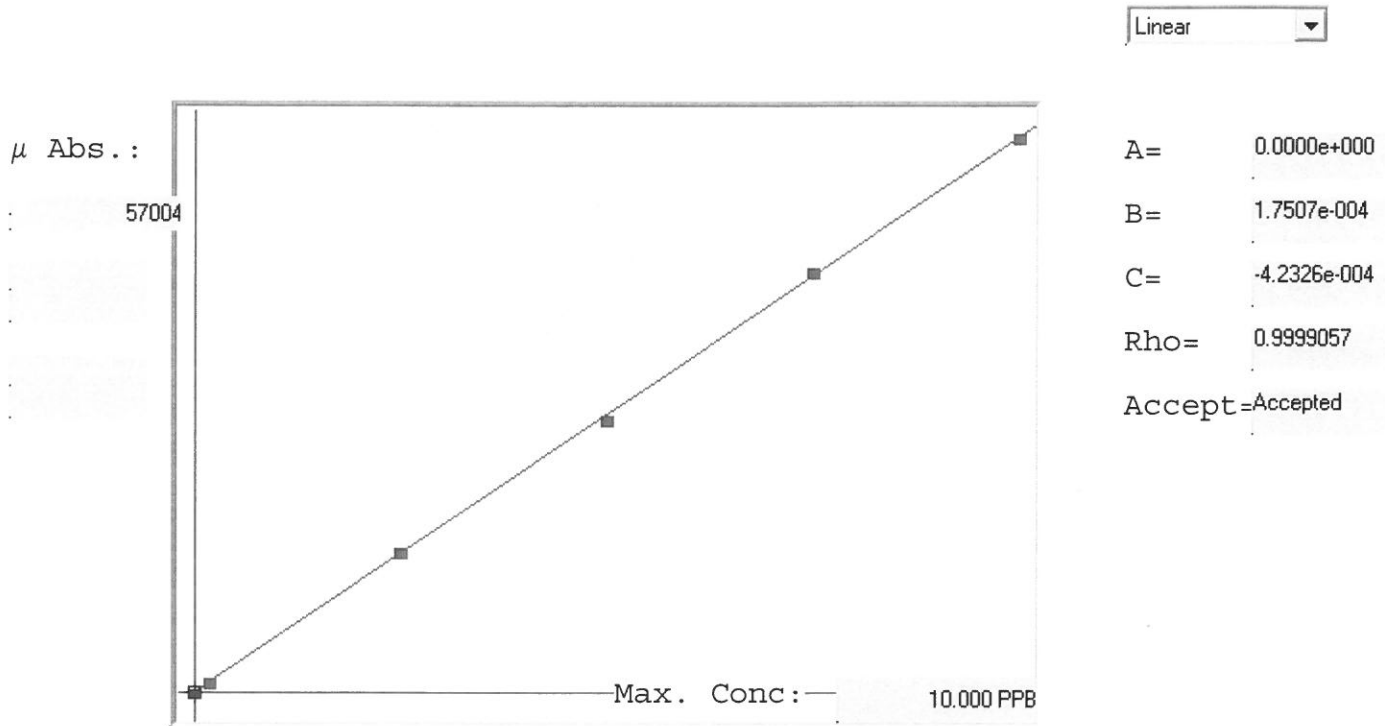

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.002	0.002	12	0.000	12				
0.2	0.200	0.196	-0.004	1122	0.0 %	1122				
2.5	2.500	2.541	0.041	14516	0.0 %	14516				
5.0	5.000	4.910	-0.090	28050	0.0 %	28050				
7.5	7.500	7.572	0.072	43256	0.0 %	43256				
10.0	10.000	9.979	-0.021	57004	0.0 %	57004				

LB108991 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 04 May 2020 10:07:43

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	SD	12	-	0.00007471B	PPB	04 May 2020 10:12:52	S	Std
0.2 - 1	SD 2	1122	-	0.20007471B	PPB	04 May 2020 10:15:09	S	Std
2.5 - 1	SD 2.5	14516	-	2.50007471B	PPB	04 May 2020 10:17:26	S	Std
5.0 - 1	SD 5	28050	-	5.00007471B	PPB	04 May 2020 10:19:43	S	Std
7.5 - 1	SD 7.5	43256	-	7.50007471B	PPB	04 May 2020 10:21:59	S	Std
10.0 - 1	SD 10	57004	-	10.00007471B	PPB	04 May 2020 10:24:16	S	Std
ICV29 - 1	ICV29	21391	3.7444	-7471B	PPB	04 May 2020 10:27:02	U	SMPL
ICB29 - 1	ICB29	-78	-0.0141	-7471B	PPB	04 May 2020 10:29:16	U	SMPL
CCV42 - 1	CCV42	28363	4.9650	-7471B	PPB	04 May 2020 10:31:32	U	SMPL
CCB42 - 1	CCB42	-69	-0.0125	-7471B	PPB	04 May 2020 10:33:47	U	SMPL
CRA - 1	CRA	1099	0.1920	-7471B	PPB	04 May 2020 10:36:02	U	SMPL
HighStd - 1	HighStd	57022	9.9822	-7471B	PPB	04 May 2020 10:38:17	U	SMPL
ChkStd - 1	ChkStd	40453	7.0815	-7471B	PPB	04 May 2020 10:40:32	U	SMPL
PB128628BL - 1	PBS	-151	-0.0269	-7471B	PPB	04 May 2020 10:42:50	U	SMPL
PB128628BS - 1	LCSS	22189	3.8841	-7471B	PPB	04 May 2020 10:45:07	U	SMPL
L2475-01 - 1	FK-SF-03-009-A	7244	1.2678	-7471B	PPB	04 May 2020 10:47:24	U	SMPL
L2475-03 - 1	FK-SF-03-009-B	5416	0.9477	-7471B	PPB	04 May 2020 10:49:40	U	SMPL
L2476-01 - 1	FK-GF-03-008-A	6495	1.1366	-7471B	PPB	04 May 2020 10:51:57	U	SMPL
L2476-03 - 1	FK-GF-03-008-B	7048	1.2334	-7471B	PPB	04 May 2020 10:54:14	U	SMPL
L2477-01 - 1	FK-0D015-03-012	694	0.1211	-7471B	PPB	04 May 2020 10:56:30	U	SMPL
CCV43 - 1	CCV43	28358	4.9641	-7471B	PPB	04 May 2020 10:58:44	U	SMPL
CCB43 - 1	CCB43	-70	-0.0127	-7471B	PPB	04 May 2020 11:00:59	U	SMPL
L2478-01 - 1	FK-0D015-03-013	855	0.1493	-7471B	PPB	04 May 2020 11:03:15	U	SMPL
L2479-01 - 1	FK-0D015-03-014	751	0.1311	-7471B	PPB	04 May 2020 11:05:31	U	SMPL
L2480-01 - 1	FK-0D015-03-015	687	0.1198	-7471B	PPB	04 May 2020 11:07:46	U	SMPL
L2480-01DUP - 1	FK-0D015-03-015DUP	694	0.1211	-7471B	PPB	04 May 2020 11:10:02	U	SMPL
L2480-01MS - 1	FK-0D015-03-015MS	21621	3.7847	-7471B	PPB	04 May 2020 11:12:18	U	SMPL
L2480-01MSD - 1	FK-0D015-03-015MSD	20197	3.5354	-7471B	PPB	04 May 2020 11:14:34	U	SMPL
L2480-01LX5 - 1		42	0.0069	-7471B	PPB	04 May 2020 11:16:50	U	SMPL
L2480-01A - 1		24362	4.2645	-7471B	PPB	04 May 2020 11:19:07	U	SMPL
CCV44 - 1	CCV44	28513	4.9912	-7471B	PPB	04 May 2020 11:21:23	U	SMPL
CCB44 - 1	CCB44	-91	-0.0164	-7471B	PPB	04 May 2020 11:23:39	U	SMPL