

LB10908P


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

40070

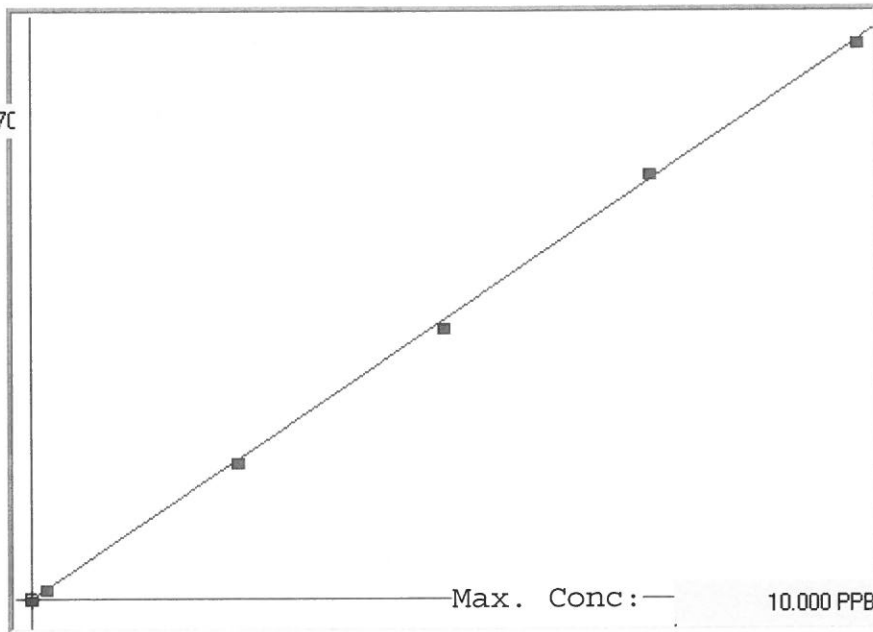

A= 0.0000e+000

B= 2.4796e-004

C= 1.9013e-002

Rho= 0.9997414

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.038	0.038	75	0.000	75				
0.2	0.200	0.217	0.017	799	0.0 %	799				
2.5	2.500	2.467	-0.033	9871	0.0 %	9871				
5.0	5.000	4.876	-0.124	19586	0.0 %	19586				
7.5	7.500	7.648	0.148	30767	0.0 %	30767				
10.0	10.000	9.955	-0.045	40070	0.0 %	40070				

LB109031 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 May 2020 14:57:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	75	-	0.0000	7470A	PPB	06 May 2020 15:00:07	S	Std
0.2 - 1	502	799	-	0.2000	7470A	PPB	06 May 2020 15:02:15	S	Std
2.5 - 1	52.5	9871	-	2.5000	7470A	PPB	06 May 2020 15:04:22	S	Std
5.0 - 1	55	19586	-	5.0000	7470A	PPB	06 May 2020 15:06:29	S	Std
7.5 - 1	57.5	30767	-	7.5000	7470A	PPB	06 May 2020 15:08:36	S	Std
10.0 - 1	310	40070	-	10.0000	7470A	PPB	06 May 2020 15:13:11	S	Std
ICV33 - 1	ICV33	16973	4.2277	-	7470A	PPB	06 May 2020 15:18:04	U	SMPL
ICB33 - 1	ICB33	-49	0.0069	-	7470A	PPB	06 May 2020 15:20:09	U	SMPL
CCV67 - 1	CCV67	20491	5.1000	-	7470A	PPB	06 May 2020 15:22:15	U	SMPL
CCB67 - 1	CCB67	-72	0.0012	-	7470A	PPB	06 May 2020 15:24:20	U	SMPL
CRA - 1	CRA	757	0.2067	-	7470A	PPB	06 May 2020 15:26:26	U	SMPL
HighStd - 1	HighStd	39712	9.8661	-	7470A	PPB	06 May 2020 15:28:32	U	SMPL
ChkStd - 1	ChkStd	27063	6.7296	-	7470A	PPB	06 May 2020 15:30:38	U	SMPL
PB128682BL - 1	PBW	-212	-0.0336	-	7470A	PPB	06 May 2020 15:32:46	U	SMPL
PB128682BS - 1	LCSW	14343	3.5755	-	7470A	PPB	06 May 2020 15:34:53	U	SMPL
L2481-21 - 1	HSM-01-W	346	0.1048	-	7470A	PPB	06 May 2020 15:37:00	U	SMPL
L2481-21DUP - 1	HSM-01-WDUP	375	0.1120	-	7470A	PPB	06 May 2020 15:39:07	U	SMPL
L2481-21MS - 1	HSM-01-WMS	15590	3.8848	-	7470A	PPB	06 May 2020 15:41:15	U	SMPL
L2481-21MSD - 1	HSM-01-WMSD	15359	3.8275	-	7470A	PPB	06 May 2020 15:43:23	U	SMPL
L2481-22 - 1	HSM-01-R	24464	6.0852	-	7470A	PPB	06 May 2020 15:45:29	U	SMPL
CCV68 - 1	CCV68	20306	5.0541	-	7470A	PPB	06 May 2020 15:47:35	U	SMPL
CCB68 - 1	CCB68	-71	0.0014	-	7470A	PPB	06 May 2020 15:49:42	U	SMPL
L2481-23 - 1	HSM-01-C	31665	7.8708	-	7470A	PPB	06 May 2020 15:51:48	U	SMPL
L2481-24 - 1	HSM-02-W	377	0.1125	-	7470A	PPB	06 May 2020 15:53:54	U	SMPL
L2481-25 - 1	HSM-02-R	5986	1.5033	-	7470A	PPB	06 May 2020 15:56:01	U	SMPL
L2481-26 - 1	HSM-02-C	4566	1.1512	-	7470A	PPB	06 May 2020 15:58:08	U	SMPL
L2481-27 - 1	HSM-03-W	304	0.0944	-	7470A	PPB	06 May 2020 16:00:15	U	SMPL
L2481-28 - 1	HSM-03-R	9438	2.3593	-	7470A	PPB	06 May 2020 16:02:22	U	SMPL
L2481-29 - 1	HSM-03-C	24811	6.1712	-	7470A	PPB	06 May 2020 16:04:29	U	SMPL
L2481-30 - 1	P-03-R	-192	-0.0286	-	7470A	PPB	06 May 2020 16:06:36	U	SMPL
L2481-31 - 1	HSM-04-W	2851	0.7260	-	7470A	PPB	06 May 2020 16:08:45	U	SMPL
L2481-32 - 1	HSM-04-R	55951	13.8928	-	7470A	PPB	06 May 2020 16:10:51	U	SMPL
CCV69 - 1	CCV69	20116	5.0070	-	7470A	PPB	06 May 2020 16:12:57	U	SMPL
CCB69 - 1	CCB69	-111	-0.0085	-	7470A	PPB	06 May 2020 16:15:05	U	SMPL
L2481-33 - 1	HSM-04-C	15641	3.8974	-	7470A	PPB	06 May 2020 16:17:11	U	SMPL
L2481-34 - 1	HSM-05-W	134	0.0522	-	7470A	PPB	06 May 2020 16:19:17	U	SMPL
L2481-35 - 1	HSM-05-R	33202	8.2519	-	7470A	PPB	06 May 2020 16:21:23	U	SMPL
L2481-36 - 1	HSM-05-C	57139	14.1874	-	7470A	PPB	06 May 2020 16:23:30	U	SMPL
L2481-37 - 1	HSM-06-W	-71	0.0014	-	7470A	PPB	06 May 2020 16:25:38	U	SMPL
L2481-38 - 1	HSM-06-R	35467	8.8135	-	7470A	PPB	06 May 2020 16:27:47	U	SMPL
L2481-39 - 1	HSM-06-C	9361	2.3402	-	7470A	PPB	06 May 2020 16:29:54	U	SMPL
L2481-40 - 1	P-03-C	203	0.0693	-	7470A	PPB	06 May 2020 16:32:03	U	SMPL
PB128683BL - 1	PBW	-57	0.0049	-	7470A	PPB	06 May 2020 16:34:10	U	SMPL
PB128683BS - 1	LCSW	13705	3.4173	-	7470A	PPB	06 May 2020 16:36:16	U	SMPL
CCV70 - 1	CCV70	19444	4.8404	-	7470A	PPB	06 May 2020 16:38:22	U	SMPL
CCB70 - 1	CCB70	-98	-0.0053	-	7470A	PPB	06 May 2020 16:40:29	U	SMPL
L2482-02 - 1	HSA-01-R	201268	49.9260	-	7470A	PPB	06 May 2020 16:42:35	U	SMPL
L2482-02DUP - 1	HSA-01-RDUP	169969	42.1650	-	7470A	PPB	06 May 2020 16:44:41	U	SMPL
L2482-02MS - 1	HSA-01-RMS	190382	47.2267	-	7470A	PPB	06 May 2020 16:46:58	U	SMPL
L2482-02MSD - 1	HSA-01-RMSD	200754	49.7986	-	7470A	PPB	06 May 2020 16:49:11	U	SMPL
L2482-04 - 1	HSA-01-C	16521	4.1156	-	7470A	PPB	06 May 2020 16:51:21	U	SMPL
L2482-06 - 1	HSA-02-R	125099	31.0389	-	7470A	PPB	06 May 2020 16:53:39	U	SMPL
L2482-08 - 1	HSA-02-C	40791	10.1337	-	7470A	PPB	06 May 2020 16:55:47	U	SMPL
L2482-10 - 1	LP-01-R	24378	6.0639	-	7470A	PPB	06 May 2020 16:57:58	U	SMPL
L2482-12 - 1	LP-01-C	931	0.2499	-	7470A	PPB	06 May 2020 17:00:07	U	SMPL
L2482-14 - 1	LP-02-R	36682	9.1148	-	7470A	PPB	06 May 2020 17:02:15	U	SMPL
CCV71 - 1	CCV71	19177	4.7742	-	7470A	PPB	06 May 2020 17:04:22	U	SMPL
CCB71 - 1	CCB71	-148	-0.0177	-	7470A	PPB	06 May 2020 17:06:29	U	SMPL
L2482-16 - 1	LP-02-C	324	0.0994	-	7470A	PPB	06 May 2020 17:08:36	U	SMPL
L2482-18 - 1	LP-03-R	8631	2.1592	-	7470A	PPB	06 May 2020 17:10:42	U	SMPL
L2482-20 - 1	LP-03-C	2481	0.6342	-	7470A	PPB	06 May 2020 17:12:48	U	SMPL
L2482-22 - 1	LW-01-R	-39	0.0093	-	7470A	PPB	06 May 2020 17:14:54	U	SMPL
L2482-24 - 1	LW-01-C	5	0.0203	-	7470A	PPB	06 May 2020 17:17:01	U	SMPL
L2482-26 - 1	LW-02-R	-2	0.0185	-	7470A	PPB	06 May 2020 17:19:08	U	SMPL
L2482-28 - 1	LW-02-C	1	0.0193	-	7470A	PPB	06 May 2020 17:21:15	U	SMPL
L2482-30 - 1	LW-03-R	0	0.0190	-	7470A	PPB	06 May 2020 17:23:22	U	SMPL
L2482-32 - 1	LW-03-C	33	0.0272	-	7470A	PPB	06 May 2020 17:25:30	U	SMPL
L2482-34 - 1	P-01-R	4	0.0200	-	7470A	PPB	06 May 2020 17:27:37	U	SMPL
CCV72 - 1	CCV72	19270	4.7973	-	7470A	PPB	06 May 2020 17:29:44	U	SMPL
CCB72 - 1	CCB72	-71	0.0014	-	7470A	PPB	06 May 2020 17:31:51	U	SMPL
L2482-36 - 1	P-01-C	-4	0.0180	-	7470A	PPB	06 May 2020 17:33:58	U	SMPL
L2482-38 - 1	P-02-R	5	0.0203	-	7470A	PPB	06 May 2020 17:36:05	U	SMPL
L2482-40 - 1	P-02-C	6	0.0205	-	7470A	PPB	06 May 2020 17:38:11	U	SMPL
PB128682TB - 1	PB128653TB	-22	0.0136	-	7470A	PPB	06 May 2020 17:40:18	U	SMPL
PB128683TB - 1	PB128666TB	-17	0.0148	-	7470A	PPB	06 May 2020 17:42:25	U	SMPL
L2481-21LX5 - 1		129	0.0510	-	7470A	PPB	06 May 2020 17:44:32	U	SMPL
L2481-21A - 1		15714	3.9155	-	7470A	PPB	06 May 2020 17:46:39	U	SMPL
L2482-02LX5 - 1		39729	9.8703	-	7470A	PPB	06 May 2020 17:48:47	U	SMPL
L2482-02A - 1		193620	48.0296	-	7470A	PPB	06 May 2020 17:50:55	U	SMPL
CCV73 - 1	CCV73	19276	4.7987	-	7470A	PPB	06 May 2020 17:53:04	U	SMPL
CCB73 - 1	CCB73	-174	-0.0241	-	7470A	PPB	06 May 2020 17:55:17	U	SMPL

LB109031 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 May 2020 14:57:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
L2481-32DLX2 - 1		27706	6.8891		-7470A	PPB	06 May 2020 17:57:24	U	SMPL
L2481-36DLX2 - 1		27884	6.9332		-7470A	PPB	06 May 2020 17:59:32	U	SMPL
L2482-02DLX10 - 1		20856	5.1905		-7470A	PPB	06 May 2020 18:01:40	U	SMPL
L2482-02DUPDLX10 - 1		21389	5.3227		-7470A	PPB	06 May 2020 18:03:48	U	SMPL
L2482-02MSDLX10 - 1		21556	5.3641		-7470A	PPB	06 May 2020 18:05:56	U	SMPL
L2482-02MSDDLX10 - 1		21595	5.3738		-7470A	PPB	06 May 2020 18:08:04	U	SMPL
L2482-02LDLX50 - 1		3647	0.9233		-7470A	PPB	06 May 2020 18:10:11	U	SMPL
L2482-02ADLX10 - 1		22536	5.6071		-7470A	PPB	06 May 2020 18:12:19	U	SMPL
L2482-06DLX10 - 1		12317	3.0732		-7470A	PPB	06 May 2020 18:15:38	U	SMPL
L2482-08DLX2 - 1		20688	5.1489		-7470A	PPB	06 May 2020 18:17:46	U	SMPL
CCV74 - 1	CCV74	19350	4.8171		-7470A	PPB	06 May 2020 18:19:53	U	SMPL
CCB74 - 1	CCB74	-113	-0.0090		-7470A	PPB	06 May 2020 18:22:01	U	SMPL