

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

5/8/2020 15:34

Reviewed by : Dh

Instrument ID : Konelab

Test: ^{Revised} ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.448	0.0	0.068	
ICB1	-0.069	0.0	0.003	
CCV1	242.922	0.0	0.164	
CCB1	-0.256	0.0	0.003	
PB128715BL	-0.363	0.0	0.003	
L2114-01	-0.482	0.0	0.003	
L2114-01DUP	-0.535	0.0	0.003	
L2497-04	-0.447	0.0	0.003	
L2498-08	-0.364	0.0	0.003	
L2513-04	-0.300	0.0	0.003	
L2515-04	-0.357	0.0	0.003	
L2523-04	-0.393	0.0	0.003	
L2525-03	-0.361	0.0	0.003	
L2530-02	-0.313	0.0	0.003	
CCV2	273.554	0.0	0.184	
CCB2	1.456	0.0	0.004	
L2531-04	-0.567	0.0	0.003	
L2531-08	-0.436	0.0	0.003	
L2554-02	-0.375	0.0	0.003	
L2554-04	-0.275	0.0	0.003	
CCV3	275.031	0.0	0.185	
CCB3	-0.314	0.0	0.003	

N 22
Mean 40.191
SD 93.4646
CV% 232.55

Aquakem v. 7.2AQ1

Results from time period:

Fri May 08 15:18:48 2020

Fri May 08 15:33:07 2020

Sh

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
ICV1	S	REACTIVE CN	P	97.4476	µg/l	5/8/2020 15:18:48
ICB1	S	REACTIVE CN	P	-0.0689	µg/l	5/8/2020 15:18:51
CCV1	S	REACTIVE CN	P	242.9222	µg/l	5/8/2020 15:18:53
CCB1	S	REACTIVE CN	P	-0.256	µg/l	5/8/2020 15:18:54
PB128715BL	S	REACTIVE CN	P	-0.3632	µg/l	5/8/2020 15:18:56
L2114-01	S	REACTIVE CN	P	-0.4821	µg/l	5/8/2020 15:18:58
L2114-01DUP	S	REACTIVE CN	P	-0.5354	µg/l	5/8/2020 15:26:20
L2497-04	S	REACTIVE CN	P	-0.4471	µg/l	5/8/2020 15:26:21
L2498-08	S	REACTIVE CN	P	-0.3635	µg/l	5/8/2020 15:26:22
L2513-04	S	REACTIVE CN	P	-0.2999	µg/l	5/8/2020 15:26:23
L2515-04	S	REACTIVE CN	P	-0.3571	µg/l	5/8/2020 15:26:24
L2523-04	S	REACTIVE CN	P	-0.3933	µg/l	5/8/2020 15:26:25
L2525-03	S	REACTIVE CN	P	-0.3606	µg/l	5/8/2020 15:26:26
L2530-02	S	REACTIVE CN	P	-0.3128	µg/l	5/8/2020 15:26:27
CCV2	S	REACTIVE CN	P	273.5537	µg/l	5/8/2020 15:26:29
CCB2	S	REACTIVE CN	P	1.456	µg/l	5/8/2020 15:26:30
L2531-04	S	REACTIVE CN	P	-0.5674	µg/l	5/8/2020 15:33:00
L2531-08	S	REACTIVE CN	P	-0.4359	µg/l	5/8/2020 15:33:01
L2554-02	S	REACTIVE CN	P	-0.3753	µg/l	5/8/2020 15:33:02
L2554-04	S	REACTIVE CN	P	-0.2753	µg/l	5/8/2020 15:33:03
CCV3	S	REACTIVE CN	P	275.0305	µg/l	5/8/2020 15:33:05
CCB3	S	REACTIVE CN	P	-0.314	µg/l	5/8/2020 15:33:06

LB109073

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dh

Instrument ID : Konelab

5/8/2020 12:27


Test ^{Result} ~~Total~~ CN

Accepted 5/8/2020 11:51

Factor 1511
Bias 0.003

Coeff. of det. 0.999893

Errors

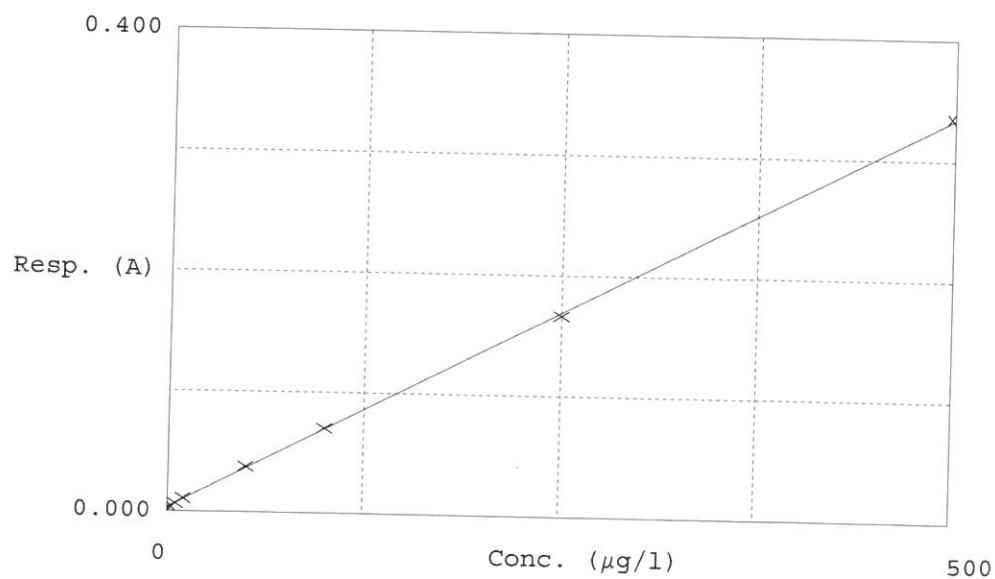

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.1665	0.0000	
2	5.0PPBCN	0.007	4.6114	5.0000	
3	10PPBCN	0.011	11.1029	10.0000	
4	50PPBCN	0.038	51.7022	50.0000	
5	100PPBCN	0.070	100.9623	100.0000	
6	250PPBCN	0.166	246.3370	250.0000	
7	500PPBCN	0.335	501.4507	500.0000	