


LB109087

7470A

INSTRUMENT ID: CV2

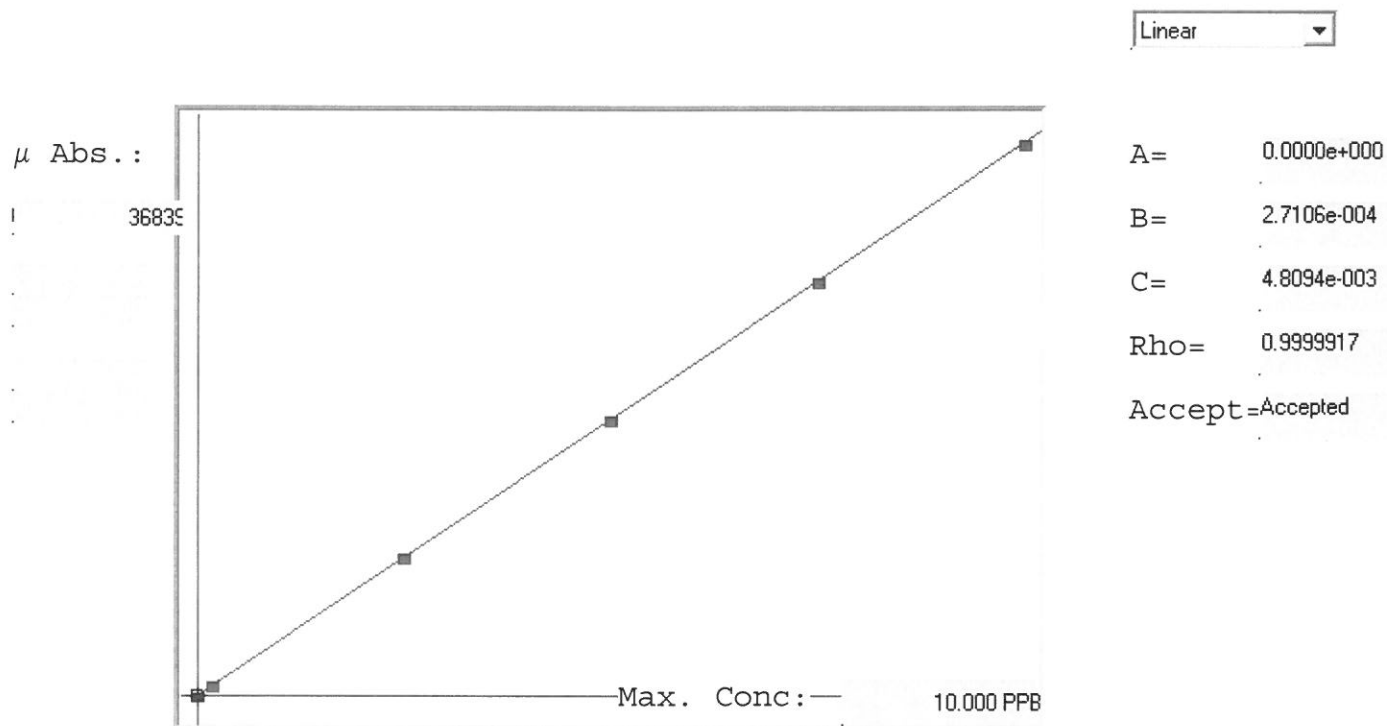

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	-27	0.000	-27				
0.2	0.200	0.181	-0.019	650	0.0 %	650				
2.5	2.500	2.529	0.029	9312	0.0 %	9312				
5.0	5.000	4.996	-0.004	18414	0.0 %	18414				
7.5	7.500	7.506	0.006	27675	0.0 %	27675				
10.0	10.000	9.990	-0.010	36839	0.0 %	36839				

LB109087 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 May 2020 10:08:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	-27	-	0.0000	7470A	PPB	11 May 2020 10:10:54	S	Std
0.2 - 1	SO.2	650	-	0.2000	7470A	PPB	11 May 2020 10:13:01	S	Std
2.5 - 1	SO.5	9312	-	2.5000	7470A	PPB	11 May 2020 10:15:09	S	Std
5.0 - 1	SE	18414	-	5.0000	7470A	PPB	11 May 2020 10:17:17	S	Std
7.5 - 1	SE.5	27675	-	7.5000	7470A	PPB	11 May 2020 10:19:23	S	Std
10.0 - 1	SIU	36839	-	10.0000	7470A	PPB	11 May 2020 10:21:29	S	Std
ICV38 - 1	ICV38	13799	3.7451	-7470A	PPB	11 May 2020 10:24:04	U	SMPL	
ICB38 - 1	ICB38	-142	-0.0337	-7470A	PPB	11 May 2020 10:26:10	U	SMPL	
CCV01 - 1	CCV01	18609	5.0489	-7470A	PPB	11 May 2020 10:28:15	U	SMPL	
CCB01 - 1	CCB01	-143	-0.0340	-7470A	PPB	11 May 2020 10:30:21	U	SMPL	
CRA - 1	CRA	667	0.1856	-7470A	PPB	11 May 2020 10:32:26	U	SMPL	
HighStd - 1	HighStd	37320	10.1206	-7470A	PPB	11 May 2020 10:34:32	U	SMPL	
ChkStd - 1	ChkStd	26487	7.1843	-7470A	PPB	11 May 2020 10:36:38	U	SMPL	
PB128762BL - 1	PBW	-208	-0.0516	-7470A	PPB	11 May 2020 10:38:46	U	SMPL	
PB128762BS - 1	LCSW	14274	3.8739	-7470A	PPB	11 May 2020 10:43:15	U	SMPL	
L2495-05 - 1	HR-05-050720	-114	-0.0261	-7470A	PPB	11 May 2020 10:45:22	U	SMPL	
L2495-05DUP - 1	HR-05-050720DUP	-35	-0.0047	-7470A	PPB	11 May 2020 10:47:29	U	SMPL	
L2495-05MS - 1	HR-05-050720MS	14284	3.8766	-7470A	PPB	11 May 2020 10:52:01	U	SMPL	
L2495-05MSD - 1	HR-05-050720MSD	14425	3.9148	-7470A	PPB	11 May 2020 10:54:08	U	SMPL	
L2503-05 - 1	OR-03-050720	-125	-0.0291	-7470A	PPB	11 May 2020 10:56:15	U	SMPL	
CCV02 - 1	CCV02	18957	5.1432	-7470A	PPB	11 May 2020 10:58:21	U	SMPL	
CCB02 - 1	CCB02	-136	-0.0321	-7470A	PPB	11 May 2020 11:00:27	U	SMPL	
L2506-05 - 1	TR-04-050720	-27	-0.0025	-7470A	PPB	11 May 2020 11:02:34	U	SMPL	
L2531-04 - 1	TP-14A	-32	-0.0039	-7470A	PPB	11 May 2020 11:04:40	U	SMPL	
L2531-08 - 1	TP-15A	-22	-0.0012	-7470A	PPB	11 May 2020 11:06:46	U	SMPL	
L2554-02 - 1	DRUM-1-7	-6	0.0032	-7470A	PPB	11 May 2020 11:08:52	U	SMPL	
L2554-04 - 1	DRUM-1-1	-7	0.0029	-7470A	PPB	11 May 2020 11:10:58	U	SMPL	
L2557-04 - 1	TP-12A	-1	0.0045	-7470A	PPB	11 May 2020 11:13:05	U	SMPL	
L2557-08 - 1	TP-13A	-5	0.0035	-7470A	PPB	11 May 2020 11:15:13	U	SMPL	
PB128762TB - 1	PB128760TB	-7	0.0029	-7470A	PPB	11 May 2020 11:17:20	U	SMPL	
L2495-05LX5 - 1		-2	0.0043	-7470A	PPB	11 May 2020 11:19:28	U	SMPL	
L2495-05A - 1		16889	4.5827	-7470A	PPB	11 May 2020 11:21:34	U	SMPL	
CCV03 - 1	CCV03	18706	5.0752	-7470A	PPB	11 May 2020 11:23:40	U	SMPL	
CCB03 - 1	CCB03	-128	-0.0299	-7470A	PPB	11 May 2020 11:25:46	U	SMPL	