


LB109204

7471B

INSTRUMENT ID: CV1

Linear

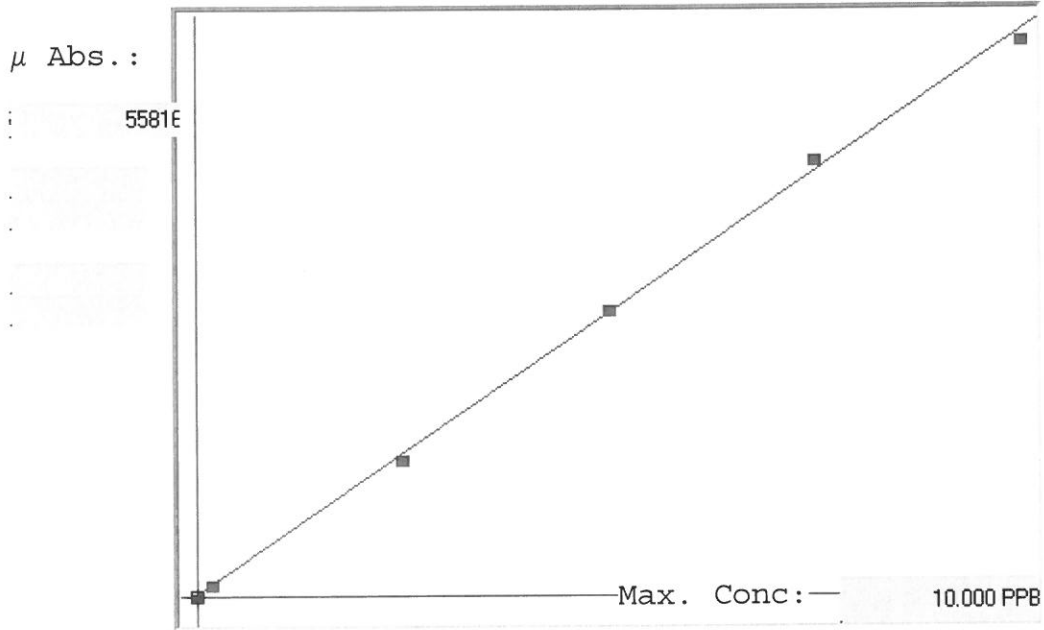

A= 0.0000e+000

B= 1.7628e-004

C= -2.1389e-002

Rho= 0.9994278

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.004	-0.004	101	0.000	101				
0.2	0.200	0.195	-0.005	1225	0.0 %	1225				
2.5	2.500	2.413	-0.087	13812	0.0 %	13812				
5.0	5.000	5.055	0.055	28798	0.0 %	28798				
7.5	7.500	7.723	0.223	43932	0.0 %	43932				
10.0	10.000	9.818	-0.182	55816	0.0 %	55816				

LB109204 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 18 May 2020 10:38:59

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	101	-	0.0000	7471B	PPB	18 May 2020 10:43:09	S	Std
0.2 - 1	50.2	1225	-	0.2000	7471B	PPB	18 May 2020 10:45:26	S	Std
2.5 - 1	52.5	13812	-	2.5000	7471B	PPB	18 May 2020 10:47:44	S	Std
5.0 - 1	55	28798	-	5.0000	7471B	PPB	18 May 2020 10:50:01	S	Std
7.5 - 1	57.5	43932	-	7.5000	7471B	PPB	18 May 2020 10:52:17	S	Std
10.0 - 1	510	55816	-	10.0000	7471B	PPB	18 May 2020 10:57:06	S	Std
ICV51 - 1	ICV51	23978	4.2054	-7471B	PPB	PPB	18 May 2020 11:02:21	U	SMPL
ICB51 - 1	ICB51	-97	-0.0385	-7471B	PPB	PPB	18 May 2020 11:04:35	U	SMPL
CCV54 - 1	CCV54	28790	5.0537	-7471B	PPB	PPB	18 May 2020 11:06:51	U	SMPL
CCB54 - 1	CCB54	-89	-0.0371	-7471B	PPB	PPB	18 May 2020 11:09:06	U	SMPL
CRA - 1	CRA	1220	0.1937	-7471B	PPB	PPB	18 May 2020 11:11:22	U	SMPL
HighStd - 1	HighStd	56382	9.9175	-7471B	PPB	PPB	18 May 2020 11:13:37	U	SMPL
ChkStd - 1	ChkStd	40147	7.0556	-7471B	PPB	PPB	18 May 2020 11:15:52	U	SMPL
PB128927BL - 1	PBS	-166	-0.0507	-7471B	PPB	PPB	18 May 2020 11:18:10	U	SMPL
PB128927BS - 1	LCSS	19328	3.3857	-7471B	PPB	PPB	18 May 2020 11:20:27	U	SMPL
L2506-08 - 1	TR-05-051520	1660	0.2712	-7471B	PPB	PPB	18 May 2020 11:22:44	U	SMPL
L2674-02 - 1	PS-STOCK-4	8661	1.5054	-7471B	PPB	PPB	18 May 2020 11:25:01	U	SMPL
L2674-02DUP - 1	PS-STOCK-4DUP	7541	1.3079	-7471B	PPB	PPB	18 May 2020 11:27:18	U	SMPL
L2674-02MS - 1	PS-STOCK-4MS	29488	5.1767	-7471B	PPB	PPB	18 May 2020 11:29:36	U	SMPL
L2674-02MSD - 1	PS-STOCK-4MSD	28054	4.9239	-7471B	PPB	PPB	18 May 2020 11:31:51	U	SMPL
CCV55 - 1	CCV55	28317	4.9703	-7471B	PPB	PPB	18 May 2020 11:34:07	U	SMPL
CCB55 - 1	CCB55	-80	-0.0355	-7471B	PPB	PPB	18 May 2020 11:36:23	U	SMPL
L2675-08 - 1	CONCRETE-PILE	13280	2.3196	-7471B	PPB	PPB	18 May 2020 11:38:38	U	SMPL
L2674-02LX5 - 1		1651	0.2696	-7471B	PPB	PPB	18 May 2020 11:40:54	U	SMPL
L2674-02A - 1		29136	5.1146	-7471B	PPB	PPB	18 May 2020 11:43:09	U	SMPL
CCV56 - 1	CCV56	28373	4.9801	-7471B	PPB	PPB	18 May 2020 11:45:24	U	SMPL
CCB56 - 1	CCB56	-82	-0.0358	-7471B	PPB	PPB	18 May 2020 11:47:41	U	SMPL