


LB109254

7471B

INSTRUMENT ID: CV1

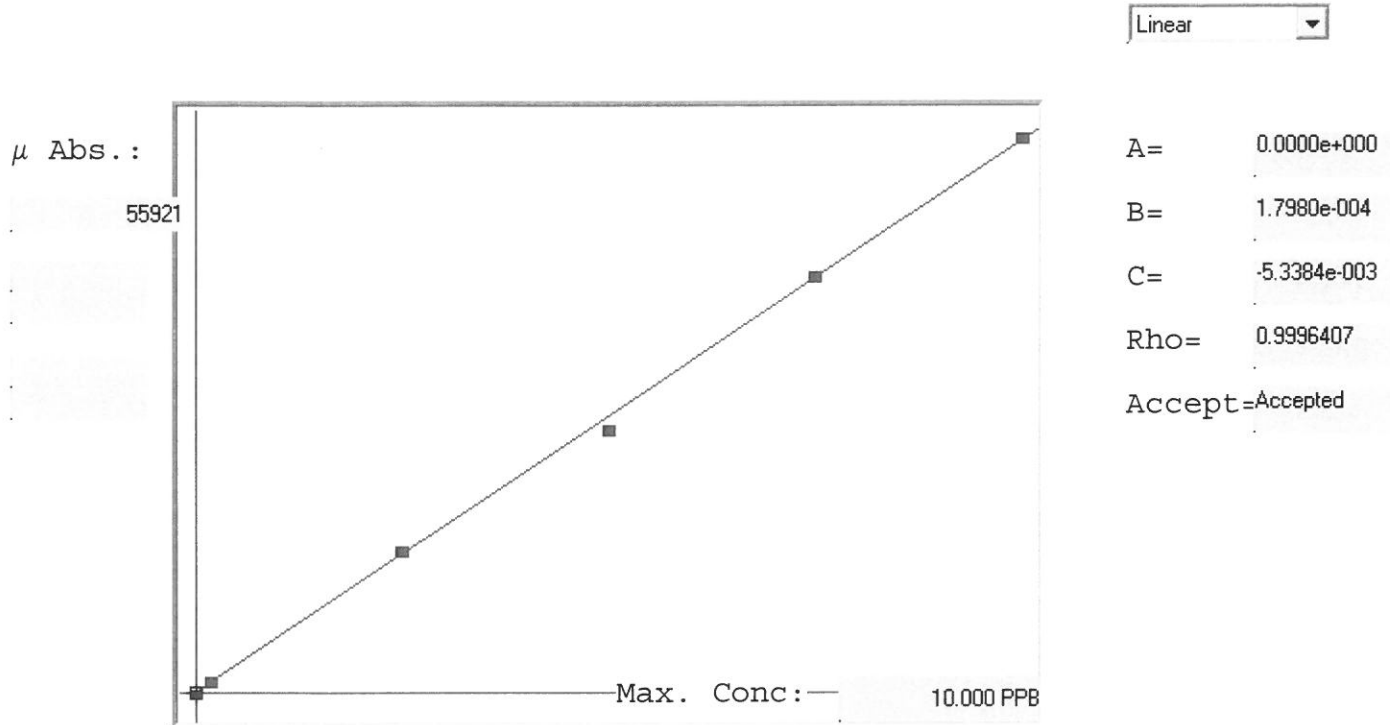

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.023	0.023	158	0.000	158				
0.2	0.200	0.224	0.024	1277	0.0 %	1277				
2.5	2.500	2.575	0.075	14352	0.0 %	14352				
5.0	5.000	4.782	-0.218	26628	0.0 %	26628				
7.5	7.500	7.546	0.046	42000	0.0 %	42000				
10.0	10.000	10.049	0.049	55921	0.0 %	55921				

LB109254 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 21 May 2020 09:23:47

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	158	-	0.00007471B	PPB		21 May 2020 09:53:09	S	Std
0.2 - 1	50.2	1277	-	0.20007471B	PPB		21 May 2020 09:55:26	S	Std
2.5 - 1	52.5	14352	-	2.50007471B	PPB		21 May 2020 09:57:44	S	Std
5.0 - 1	55	26628	-	5.00007471B	PPB		21 May 2020 10:00:01	S	Std
7.5 - 1	57.5	42000	-	7.50007471B	PPB		21 May 2020 10:02:17	S	Std
10.0 - 1	510	55921	-	10.00007471B	PPB		21 May 2020 10:04:34	S	Std
ICV56 - 1	ICV56	22336	4.0106	-7471B	PPB		21 May 2020 10:07:30	U	SMPL
ICB56 - 1	ICB56	56	0.0047	-7471B	PPB		21 May 2020 10:09:44	U	SMPL
CCV82 - 1	CCV82	27981	5.0256	-7471B	PPB		21 May 2020 10:12:00	U	SMPL
CCB82 - 1	CCB82	53	0.0042	-7471B	PPB		21 May 2020 10:14:14	U	SMPL
CRA - 1	CRA	1270	0.2230	-7471B	PPB		21 May 2020 10:16:31	U	SMPL
HighStd - 1	HighStd	56173	10.0944	-7471B	PPB		21 May 2020 10:18:46	U	SMPL
ChkStd - 1	ChkStd	39885	7.1659	-7471B	PPB		21 May 2020 10:21:02	U	SMPL
PB129028BL - 1	PBS	-33	-0.0113	-7471B	PPB		21 May 2020 10:23:19	U	SMPL
PB129028BS - 1	LCSS	20845	3.7425	-7471B	PPB		21 May 2020 10:25:37	U	SMPL
L2506-14 - 1	TR-04-052020	4321	0.7716	-7471B	PPB		21 May 2020 10:27:53	U	SMPL
L2506-14DUP - 1	TR-04-052020DUP	3959	0.7065	-7471B	PPB		21 May 2020 10:30:10	U	SMPL
L2506-14MS - 1	TR-04-052020MS	24168	4.3400	-7471B	PPB		21 May 2020 10:35:20	U	SMPL
L2506-14MSD - 1	TR-04-052020MSD	23138	4.1548	-7471B	PPB		21 May 2020 10:37:37	U	SMPL
L2717-01 - 1	DRUM-01-04	-42	-0.0129	-7471B	PPB		21 May 2020 10:39:54	U	SMPL
CCV83 - 1	CCV83	27988	5.0268	-7471B	PPB		21 May 2020 10:42:10	U	SMPL
CCB83 - 1	CCB83	74	0.0080	-7471B	PPB		21 May 2020 10:44:25	U	SMPL
L2718-01 - 1	72-12017	2353	0.4177	-7471B	PPB		21 May 2020 10:46:42	U	SMPL
L2719-01 - 1	AOC-17	2013	0.3566	-7471B	PPB		21 May 2020 10:48:57	U	SMPL
L2722-01 - 1	COMP-1	996	0.1737	-7471B	PPB		21 May 2020 10:51:13	U	SMPL
L2722-02 - 1	COMP-2	1263	0.2217	-7471B	PPB		21 May 2020 10:53:28	U	SMPL
L2722-03 - 1	COMP-3	514	0.0871	-7471B	PPB		21 May 2020 10:55:44	U	SMPL
L2728-01 - 1	239994	1056	0.1845	-7471B	PPB		21 May 2020 10:58:01	U	SMPL
L2728-04 - 1	239990	18419	3.3063	-7471B	PPB		21 May 2020 11:00:17	U	SMPL
L2728-07 - 1	239998	3223	0.5741	-7471B	PPB		21 May 2020 11:02:34	U	SMPL
L2728-10 - 1	240000	1514	0.2669	-7471B	PPB		21 May 2020 11:04:50	U	SMPL
L2728-13 - 1	240001	1561	0.2753	-7471B	PPB		21 May 2020 11:07:06	U	SMPL
CCV84 - 1	CCV84	28555	5.1288	-7471B	PPB		21 May 2020 11:09:21	U	SMPL
CCB84 - 1	CCB84	59	0.0053	-7471B	PPB		21 May 2020 11:11:37	U	SMPL
L2506-14LX5 - 1		844	0.1464	-7471B	PPB		21 May 2020 11:13:53	U	SMPL
L2506-14A - 1		24291	4.3621	-7471B	PPB		21 May 2020 11:16:09	U	SMPL
CCV85 - 1	CCV85	28436	5.1074	-7471B	PPB		21 May 2020 11:18:24	U	SMPL
CCB85 - 1	CCB85	60	0.0054	-7471B	PPB		21 May 2020 11:20:40	U	SMPL