


LB109283

7470A

INSTRUMENT ID: CX1

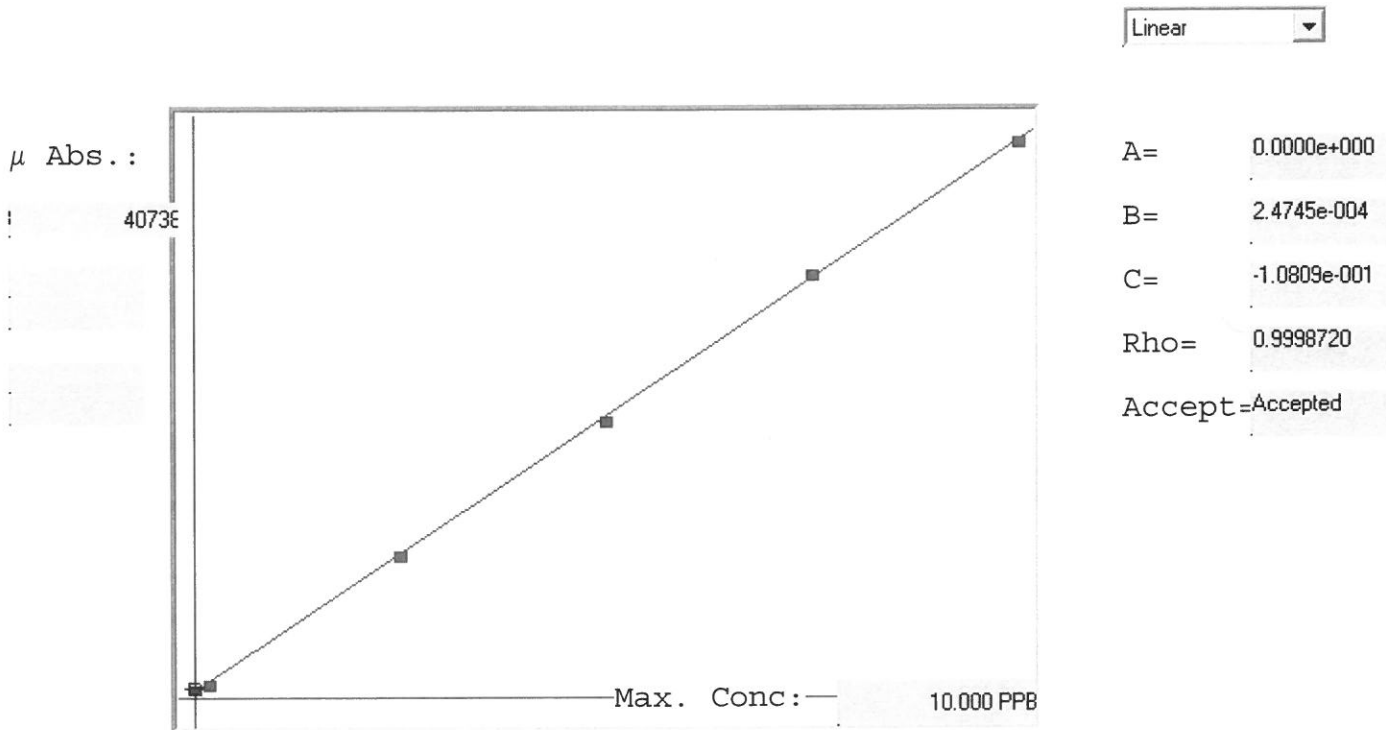

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.067	0.067	707	0.000	707				
0.2	0.200	0.147	-0.053	1032	0.0 %	1032				
2.5	2.500	2.505	0.005	10561	0.0 %	10561				
5.0	5.000	4.924	-0.076	20335	0.0 %	20335				
7.5	7.500	7.584	0.084	31086	0.0 %	31086				
10.0	10.000	9.973	-0.027	40738	0.0 %	40738				

Report Title

Method: 7470A

Operator: Admin

Date of Analysis: 22 May 2020 14:03:28

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	707	-	0.0000	7470A	PPB	22 May 2020 14:12:32	S	Std
0.2 - 1	50.2	1032	-	0.2000	7470A	PPB	22 May 2020 14:14:40	S	Std
2.5 - 1	52.5	10561	-	2.5000	7470A	PPB	22 May 2020 14:16:48	S	Std
5.0 - 1	55	20335	-	5.0000	7470A	PPB	22 May 2020 14:18:56	S	Std
7.5 - 1	57.5	31086	-	7.5000	7470A	PPB	22 May 2020 14:21:02	S	Std
10.0 - 1	510	40738	-	10.0000	7470A	PPB	22 May 2020 14:25:41	S	Std
ICV58 - 1	ICV58	15761	3.7920	-	7470A	PPB	22 May 2020 14:28:14	U	SMPL
ICB58 - 1	ICB58	489	0.0129	-	7470A	PPB	22 May 2020 14:30:20	U	SMPL
CCV91 - 1	CCV91	20406	4.9414	-	7470A	PPB	22 May 2020 14:32:26	U	SMPL
CCB91 - 1	CCB91	475	0.0094	-	7470A	PPB	22 May 2020 14:34:31	U	SMPL
CRA - 1	CRA	1038	0.1488	-	7470A	PPB	22 May 2020 14:36:37	U	SMPL
HighStd - 1	HighStd	40359	9.8788	-	7470A	PPB	22 May 2020 14:38:42	U	SMPL
ChkStd - 1	ChkStd	28193	6.8683	-	7470A	PPB	22 May 2020 14:40:48	U	SMPL
PB129067BL - 1	PBW	395	-0.0103	-	7470A	PPB	22 May 2020 14:53:22	U	SMPL
PB129067BS - 1	LCSW	14634	3.5131	-	7470A	PPB	22 May 2020 14:55:28	U	SMPL
L2738-13 - 1	1702	959	0.1292	-	7470A	PPB	22 May 2020 14:57:35	U	SMPL
L2738-16 - 1	1723	119	-0.0786	-	7470A	PPB	22 May 2020 14:59:43	U	SMPL
L2738-16DUP - 1	1723DUP	135	-0.0747	-	7470A	PPB	22 May 2020 15:01:50	U	SMPL
L2738-16MS - 1	1723MS	12407	2.9620	-	7470A	PPB	22 May 2020 15:03:58	U	SMPL
L2738-16MSD - 1	1723MSD	12280	2.9306	-	7470A	PPB	22 May 2020 15:06:05	U	SMPL
CCV92 - 1	CCV92	20630	4.9968	-	7470A	PPB	22 May 2020 15:13:02	U	SMPL
CCB92 - 1	CCB92	435	-0.0004	-	7470A	PPB	22 May 2020 15:15:08	U	SMPL
PB129068BL - 1	PBW	58	-0.0937	-	7470A	PPB	22 May 2020 15:17:15	U	SMPL
PB129068BS - 1	LCSW	13999	3.3560	-	7470A	PPB	22 May 2020 15:19:21	U	SMPL
L2738-04 - 1	25-28-COMP	545	0.0268	-	7470A	PPB	22 May 2020 15:21:26	U	SMPL
L2738-04DUP - 1	25-28-COMPDUP	70	-0.0908	-	7470A	PPB	22 May 2020 15:23:33	U	SMPL
L2738-04MS - 1	25-28-COMPMS	11943	2.8472	-	7470A	PPB	22 May 2020 15:25:39	U	SMPL
L2738-04MSD - 1	25-28-COMPMSD	11872	2.8297	-	7470A	PPB	22 May 2020 15:27:46	U	SMPL
CCV93 - 1	CCV93	21024	5.0943	-	7470A	PPB	22 May 2020 15:32:59	U	SMPL
CCB93 - 1	CCB93	418	-0.0047	-	7470A	PPB	22 May 2020 15:35:06	U	SMPL
PB129067TB - 1	PB129053TB	67	-0.0915	-	7470A	PPB	22 May 2020 15:38:14	U	SMPL
PB129068TB - 1	PB129054TB	354	-0.0205	-	7470A	PPB	22 May 2020 15:40:20	U	SMPL
L2738-16LX5 - 1		587	0.0372	-	7470A	PPB	22 May 2020 15:42:26	U	SMPL
L2738-16A - 1		14367	3.4470	-	7470A	PPB	22 May 2020 15:47:15	U	SMPL
L2738-04LX5 - 1		498	0.0151	-	7470A	PPB	22 May 2020 15:49:21	U	SMPL
L2738-04A - 1		14056	3.3701	-	7470A	PPB	22 May 2020 15:51:27	U	SMPL
CCV94 - 1	CCV94	20976	5.0825	-	7470A	PPB	22 May 2020 15:53:33	U	SMPL
CCB94 - 1	CCB94	407	-0.0074	-	7470A	PPB	22 May 2020 15:55:39	U	SMPL