

LB 109313

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : du

Instrument ID : Konelab

5/26/2020 13:24

Test: ^{Residue} Total CN

Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.351	0.0	0.077	
ICB1	-0.508	0.0	0.004	
CCV1	243.524	0.0	0.192	
CCB1	0.068	0.0	0.004	
PB129093BL	-0.238	0.0	0.004	
L2498-16	-0.342	0.0	0.004	
L2498-16DUP	-0.686	0.0	0.004	
L2500-10	-0.667	0.0	0.004	
L2757-04	-0.641	0.0	0.004	
L2757-05	-0.446	0.0	0.004	
L2757-06	-0.372	0.0	0.004	
CCV2	242.030	0.0	0.191	
CCB2	-0.346	0.0	0.004	

N	13
Mean	44.287
SD	91.8739
CV%	207.45

Aquakem v. 7.2AQ1

Results from time period:

Tue May 26 13:05:59 2020

Tue May 26 13:13:15 2020

De

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	-1.1351	µg/l	5/26/2020 10:42:14	
5.OPPBCN	A	REACTIVE CN	P	4.3046	µg/l	5/26/2020 10:42:15	
10PPBCN	A	REACTIVE CN	P	9.1314	µg/l	5/26/2020 10:42:16	
50PPBCN	A	REACTIVE CN	P	49.7826	µg/l	5/26/2020 10:42:17	
100PPBCN	A	REACTIVE CN	P	102.658	µg/l	5/26/2020 10:42:18	
250PPBCN	A	REACTIVE CN	P	251.4881	µg/l	5/26/2020 10:42:19	
500PPBCN	A	REACTIVE CN	P	498.7704	µg/l	5/26/2020 10:42:20	
ICV1	S	REACTIVE CN	P	94.3509	µg/l	5/26/2020 13:06:00	
ICB1	S	REACTIVE CN	P	-0.5082	µg/l	5/26/2020 13:06:01	
CCV1	S	REACTIVE CN	P	243.5245	µg/l	5/26/2020 13:06:04	
CCB1	S	REACTIVE CN	P	0.0677	µg/l	5/26/2020 13:06:05	
PB129093BL	S	REACTIVE CN	P	-0.2381	µg/l	5/26/2020 13:06:07	
L2498-16	S	REACTIVE CN	P	-0.3425	µg/l	5/26/2020 13:06:09	
L2498-16DUP	S	REACTIVE CN	P	-0.686	µg/l	5/26/2020 13:13:07	
L2500-10	S	REACTIVE CN	P	-0.6674	µg/l	5/26/2020 13:13:08	
L2757-04	S	REACTIVE CN	P	-0.6414	µg/l	5/26/2020 13:13:09	
L2757-05	S	REACTIVE CN	P	-0.4459	µg/l	5/26/2020 13:13:10	
L2757-06	S	REACTIVE CN	P	-0.3719	µg/l	5/26/2020 13:13:11	
CCV2	S	REACTIVE CN	P	242.0295	µg/l	5/26/2020 13:13:13	
CCB2	S	REACTIVE CN	P	-0.3459	µg/l	5/26/2020 13:13:14	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : 174

Instrument ID : Konelab

5/26/2020 13:38


Test ~~Total~~ ^{Positive} CN

Accepted 5/26/2020 10:43

Factor 1298
Bias 0.004

Coeff. of det. 0.999935

Errors

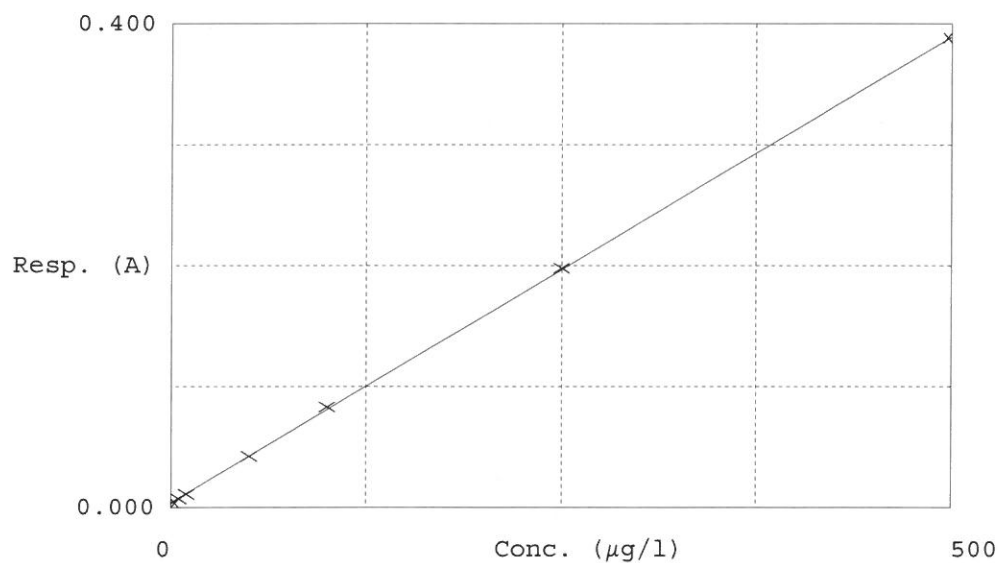

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.1351	0.0000	
2	5.0PPBCN	0.007	4.3046	5.0000	
3	10PPBCN	0.011	9.1314	10.0000	
4	50PPBCN	0.042	49.7826	50.0000	
5	100PPBCN	0.083	102.6580	100.0000	
6	250PPBCN	0.198	251.4881	250.0000	
7	500PPBCN	0.388	498.7704	500.0000	