


LB109314

7470A

INSTRUMENT ID: CV2

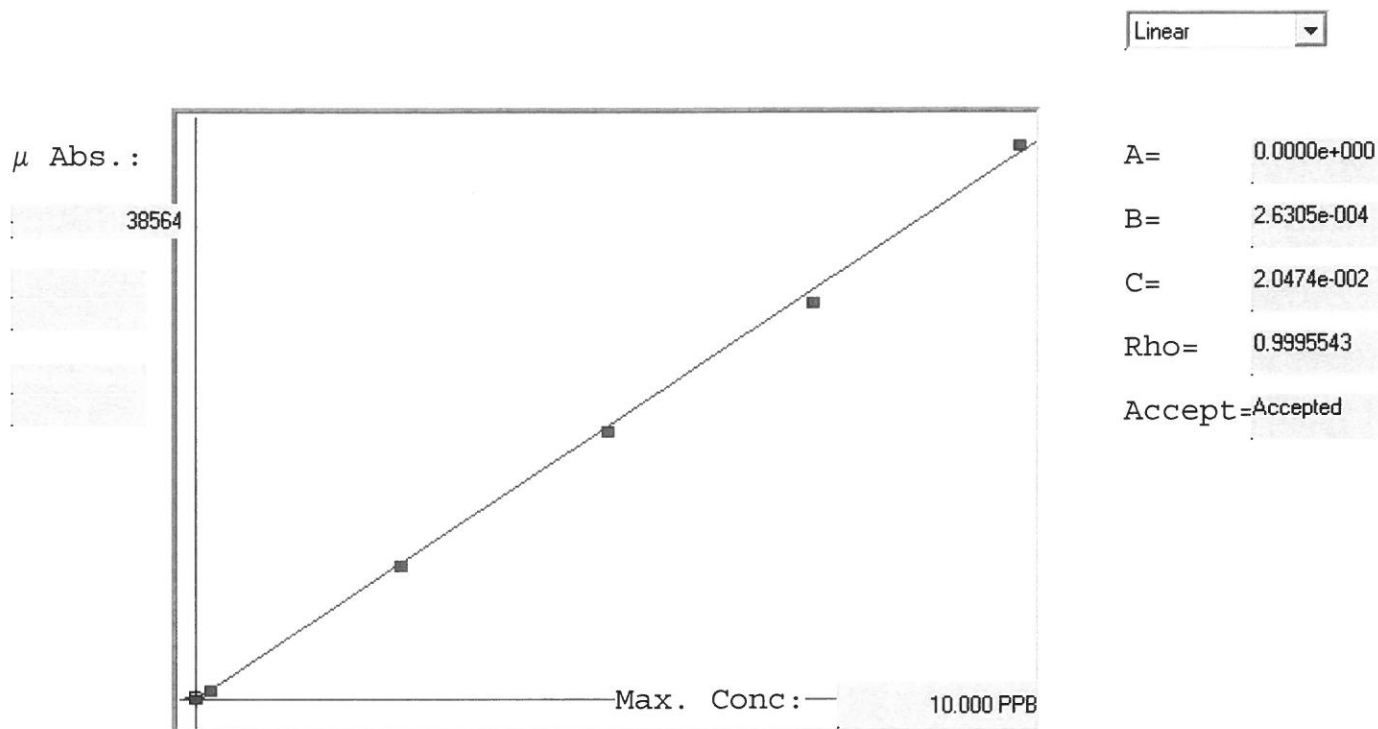

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.056	0.056	135	0.000	135				
0.2	0.200	0.226	0.026	783	0.0 %	783				
2.5	2.500	2.497	-0.003	9413	0.0 %	9413				
5.0	5.000	4.956	-0.044	18761	0.0 %	18761				
7.5	7.500	7.300	-0.200	27675	0.0 %	27675				
10.0	10.000	10.165	0.165	38564	0.0 %	38564				

LB109314 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 May 2020 13:48:26

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50	135	-	0.0000	7470A	PPB	26 May 2020 13:54:21	S	Std
0.2 - 1	50.2	783	-	0.2000	7470A	PPB	26 May 2020 13:56:29	S	Std
2.5 - 1	52.5	9413	-	2.5000	7470A	PPB	26 May 2020 13:58:37	S	Std
5.0 - 1	55	18761	-	5.0000	7470A	PPB	26 May 2020 14:00:45	S	Std
7.5 - 1	57.5	27675	-	7.5000	7470A	PPB	26 May 2020 14:02:52	S	Std
10.0 - 1	51.8	38564	-	10.0000	7470A	PPB	26 May 2020 14:07:48	S	Std
ICV59 - 1	ICV59	14138	3.7395	-	7470A	PPB	26 May 2020 14:10:21	U	SMPL
ICB59 - 1	ICB59	89	0.0439	-	7470A	PPB	26 May 2020 14:12:27	U	SMPL
CCV95 - 1	CCV95	18647	4.9256	-	7470A	PPB	26 May 2020 14:14:33	U	SMPL
CCB95 - 1	CCB95	64	0.0373	-	7470A	PPB	26 May 2020 14:16:38	U	SMPL
CRA - 1	CRA	761	0.2207	-	7470A	PPB	26 May 2020 14:18:44	U	SMPL
HighStd - 1	HighStd	38132	10.0512	-	7470A	PPB	26 May 2020 14:20:50	U	SMPL
ChkStd - 1	ChkStd	26114	6.8899	-	7470A	PPB	26 May 2020 14:22:55	U	SMPL
PB129087BL - 1	PBW	-70	0.0021	-	7470A	PPB	26 May 2020 14:25:03	U	SMPL
PB129087BS - 1	LCSW	14161	3.7456	-	7470A	PPB	26 May 2020 14:27:11	U	SMPL
L2498-16 - 1	CL-01-052220	-13	0.0171	-	7470A	PPB	26 May 2020 14:29:18	U	SMPL
L2498-16DUP - 1	CL-01-052220DUP	58	0.0357	-	7470A	PPB	26 May 2020 14:31:25	U	SMPL
L2498-16MS - 1	CL-01-052220MS	14339	3.7924	-	7470A	PPB	26 May 2020 14:33:33	U	SMPL
L2498-16MSD - 1	CL-01-052220MSD	15275	4.0386	-	7470A	PPB	26 May 2020 14:35:41	U	SMPL
L2500-10 - 1	OK-03-052220	2	0.0210	-	7470A	PPB	26 May 2020 14:37:47	U	SMPL
CCV96 - 1	CCV96	18667	4.9309	-	7470A	PPB	26 May 2020 14:39:54	U	SMPL
CCB96 - 1	CCB96	81	0.0418	-	7470A	PPB	26 May 2020 14:42:00	U	SMPL
PB129088BL - 1	PBW	78	0.0410	-	7470A	PPB	26 May 2020 14:44:05	U	SMPL
PB129088BS - 1	LCSW	15018	3.9710	-	7470A	PPB	26 May 2020 14:46:12	U	SMPL
L2744-25 - 1	NM-EB-1	-116	-0.0100	-	7470A	PPB	26 May 2020 14:48:18	U	SMPL
L2745-21 - 1	NM-EB-2	-56	0.0057	-	7470A	PPB	26 May 2020 14:50:25	U	SMPL
L2745-22 - 1	NM-EB-3	-57	0.0055	-	7470A	PPB	26 May 2020 14:52:31	U	SMPL
L2746-20 - 1	NM-EB-4	-73	0.0013	-	7470A	PPB	26 May 2020 14:54:38	U	SMPL
L2747-01 - 1	MW-14	-60	0.0047	-	7470A	PPB	26 May 2020 14:56:45	U	SMPL
L2747-02 - 1	SW-2	-71	0.0018	-	7470A	PPB	26 May 2020 14:58:53	U	SMPL
L2747-02DUP - 1	SW-2DUP	-49	0.0076	-	7470A	PPB	26 May 2020 15:01:00	U	SMPL
L2747-03 - 1	MW-6R	265	0.0902	-	7470A	PPB	26 May 2020 15:03:07	U	SMPL
CCV97 - 1	CCV97	18825	4.9725	-	7470A	PPB	26 May 2020 15:05:13	U	SMPL
CCB97 - 1	CCB97	72	0.0394	-	7470A	PPB	26 May 2020 15:07:20	U	SMPL
L2747-04 - 1	MW-9R	-12	0.0173	-	7470A	PPB	26 May 2020 15:09:26	U	SMPL
L2747-05 - 1	MW-8R	8	0.0226	-	7470A	PPB	26 May 2020 15:11:33	U	SMPL
L2747-06 - 1	SW-3	-49	0.0076	-	7470A	PPB	26 May 2020 15:13:39	U	SMPL
L2747-07 - 1	SW-1	-70	0.0021	-	7470A	PPB	26 May 2020 15:15:45	U	SMPL
L2747-08 - 1	SW-2-DUP	-41	0.0097	-	7470A	PPB	26 May 2020 15:17:51	U	SMPL
L2747-09 - 1	L2747-02MS	14323	3.7882	-	7470A	PPB	26 May 2020 15:19:59	U	SMPL
L2747-10 - 1	L2747-02MSD	14322	3.7879	-	7470A	PPB	26 May 2020 15:22:06	U	SMPL
CCV98 - 1	CCV98	19156	5.0595	-	7470A	PPB	26 May 2020 15:24:14	U	SMPL
CCB98 - 1	CCB98	101	0.0470	-	7470A	PPB	26 May 2020 15:26:22	U	SMPL
L2498-16LX5 - 1		108	0.0489	-	7470A	PPB	26 May 2020 15:28:28	U	SMPL
L2498-16A - 1		15002	3.9668	-	7470A	PPB	26 May 2020 15:30:34	U	SMPL
L2747-02LX5 - 1		42	0.0315	-	7470A	PPB	26 May 2020 15:32:41	U	SMPL
L2747-02A - 1		14583	3.8566	-	7470A	PPB	26 May 2020 15:37:09	U	SMPL
PB129087TB - 1	PB129073TB	21	0.0260	-	7470A	PPB	26 May 2020 15:39:15	U	SMPL
CCV99 - 1	CCV99	19386	5.1200	-	7470A	PPB	26 May 2020 15:41:21	U	SMPL
CCB99 - 1	CCB99	58	0.0357	-	7470A	PPB	26 May 2020 15:43:27	U	SMPL