


LB109338
INSTRUMENT ID: Cx1

7470A

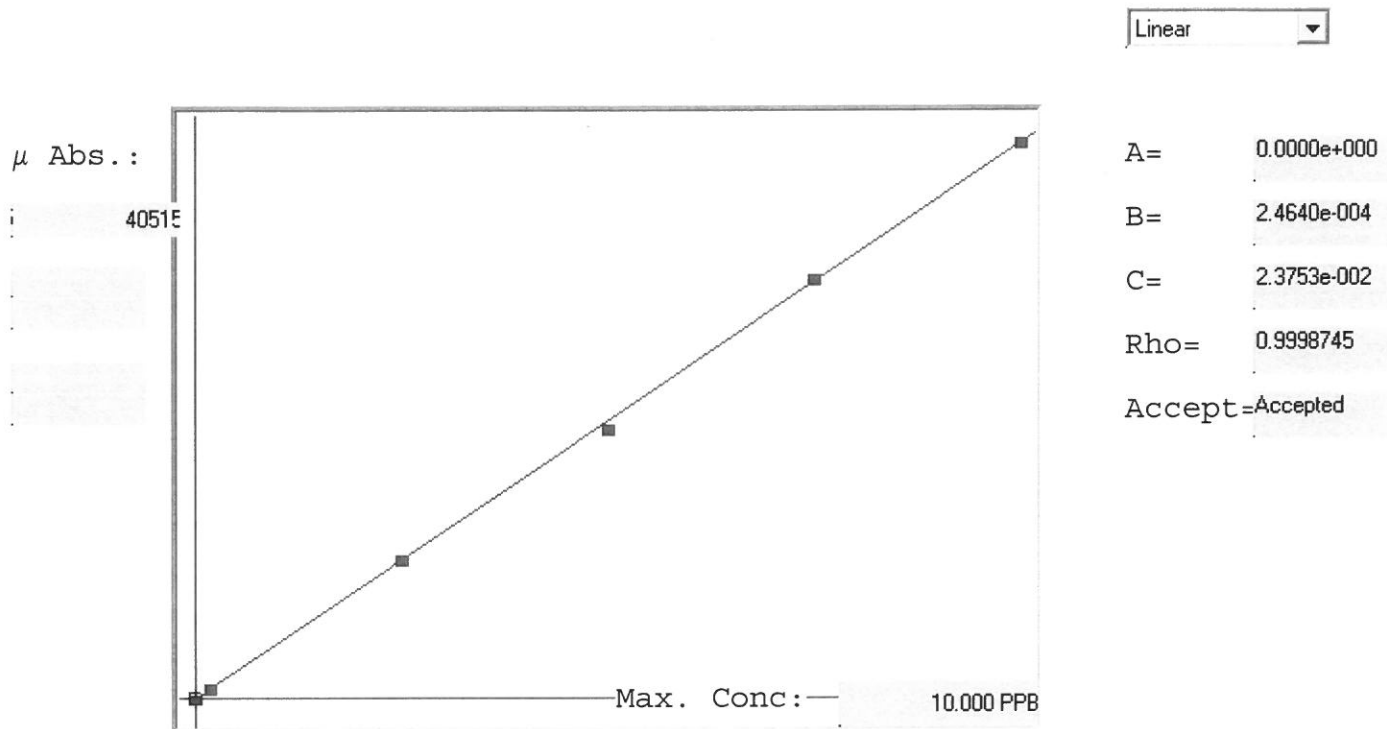

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.036	0.036	50	0.000	50				
0.2	0.200	0.199	-0.001	713	0.0 %	713				
2.5	2.500	2.515	0.015	10110	0.0 %	10110				
5.0	5.000	4.878	-0.122	19703	0.0 %	19703				
7.5	7.500	7.565	0.065	30605	0.0 %	30605				
10.0	10.000	10.006	0.006	40515	0.0 %	40515				

LB109338 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 28 May 2020 09:36:09					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	50	-	0.0000	7470A	PPB	28 May 2020 09:39:12	S	Std
0.2 - 1	50.2	713	-	0.2000	7470A	PPB	28 May 2020 09:41:20	S	Std
2.5 - 1	52.5	10110	-	2.5000	7470A	PPB	28 May 2020 09:43:27	S	Std
5.0 - 1	55	19703	-	5.0000	7470A	PPB	28 May 2020 09:45:35	S	Std
7.5 - 1	57.5	30605	-	7.5000	7470A	PPB	28 May 2020 09:47:42	S	Std
10.0 - 1	51.1	40515	-	10.0000	7470A	PPB	28 May 2020 09:49:49	S	Std
ICV61 - 1	ICV61	14772	3.6635	-	7470A	PPB	28 May 2020 09:52:31	U	SMPL
ICB61 - 1	ICB61	-60	0.0090	-	7470A	PPB	28 May 2020 09:54:37	U	SMPL
CCV13 - 1	CCV13	18904	4.6816	-	7470A	PPB	28 May 2020 09:59:05	U	SMPL
CCB13 - 1	CCB13	-69	0.0068	-	7470A	PPB	28 May 2020 10:01:11	U	SMPL
CRA - 1	CRA	696	0.1952	-	7470A	PPB	28 May 2020 10:03:16	U	SMPL
HighStd - 1	HighStd	40535	10.0114	-	7470A	PPB	28 May 2020 10:05:22	U	SMPL
ChkStd - 1	ChkStd	27108	6.7031	-	7470A	PPB	28 May 2020 10:07:28	U	SMPL
PB129132BL - 1	PBW	-104	-0.0019	-	7470A	PPB	28 May 2020 10:09:36	U	SMPL
PB129132BS - 1	LCSW	15138	3.7537	-	7470A	PPB	28 May 2020 10:11:42	U	SMPL
L2767-01 - 1	TRE-1005	-55	0.0102	-	7470A	PPB	28 May 2020 10:13:49	U	SMPL
L2768-02 - 1	370	-14	0.0203	-	7470A	PPB	28 May 2020 10:15:57	U	SMPL
L2768-02DUP - 1	370DUP	8	0.0257	-	7470A	PPB	28 May 2020 10:18:04	U	SMPL
L2768-02MS - 1	370MS	13944	3.4595	-	7470A	PPB	28 May 2020 10:20:12	U	SMPL
L2768-02MSD - 1	370MSD	14505	3.5977	-	7470A	PPB	28 May 2020 10:22:18	U	SMPL
CCV14 - 1	CCV14	19782	4.8980	-	7470A	PPB	28 May 2020 10:24:24	U	SMPL
CCB14 - 1	CCB14	-84	0.0031	-	7470A	PPB	28 May 2020 10:26:30	U	SMPL
L2768-04 - 1	371	-16	0.0198	-	7470A	PPB	28 May 2020 10:28:37	U	SMPL
PB129133BL - 1	PBW	10	0.0262	-	7470A	PPB	28 May 2020 10:30:42	U	SMPL
PB129133BS - 1	LCSW	14325	3.5534	-	7470A	PPB	28 May 2020 10:32:49	U	SMPL
L2767-03 - 1	TRE-1006	230	0.0804	-	7470A	PPB	28 May 2020 10:34:55	U	SMPL
L2767-03DUP - 1	TRE-1006DUP	274	0.0913	-	7470A	PPB	28 May 2020 10:37:02	U	SMPL
L2767-03MS - 1	TRE-1006MS	14213	3.5258	-	7470A	PPB	28 May 2020 10:39:09	U	SMPL
L2767-03MSD - 1	TRE-1006MSD	14597	3.6204	-	7470A	PPB	28 May 2020 10:41:15	U	SMPL
CCV15 - 1	CCV15	19880	4.9221	-	7470A	PPB	28 May 2020 10:43:23	U	SMPL
CCB15 - 1	CCB15	-91	0.0013	-	7470A	PPB	28 May 2020 10:45:31	U	SMPL
PB129132TB - 1	PB129125TB	-10	0.0213	-	7470A	PPB	28 May 2020 10:47:37	U	SMPL
PB129133TB - 1	PB129127TB	-13	0.0206	-	7470A	PPB	28 May 2020 10:49:43	U	SMPL
L2768-02LX5 - 1		18	0.0282	-	7470A	PPB	28 May 2020 10:51:50	U	SMPL
L2768-02A - 1		17443	4.3216	-	7470A	PPB	28 May 2020 10:53:56	U	SMPL
L2767-03LX5 - 1		-2	0.0233	-	7470A	PPB	28 May 2020 10:56:02	U	SMPL
L2767-03A - 1		16639	4.1235	-	7470A	PPB	28 May 2020 10:58:08	U	SMPL
CCV16 - 1	CCV16	19388	4.8009	-	7470A	PPB	28 May 2020 11:00:14	U	SMPL
CCB16 - 1	CCB16	-113	-0.0041	-	7470A	PPB	28 May 2020 11:02:21	U	SMPL