

L15109402

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DA

Instrument ID : Konelab

6/2/2020 12:34

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.833	0.0	0.084	
ICB1	0.011	0.0	0.003	
CCV1	242.120	0.0	0.204	
CCB1	-0.044	0.0	0.003	
PB129215BL	-0.164	0.0	0.003	
L2805-02	-0.154	0.0	0.003	
L2805-02DUP	-0.104	0.0	0.003	
L2813-06	0.052	0.0	0.003	
L2814-06	0.115	0.0	0.003	
L2822-04	0.039	0.0	0.003	
L2822-05	0.186	0.0	0.003	
L2822-06	0.083	0.0	0.003	
PB129240BL	0.138	0.0	0.003	
L2831-01	0.102	0.0	0.003	
CCV2	238.590	0.0	0.201	
CCB2	0.139	0.0	0.003	
L2831-01DUP	0.145	0.0	0.003	
CCV3	243.826	0.0	0.205	
CCB3	0.375	0.0	0.004	

N	19
Mean	43.278
SD	90.9176
CV%	210.08

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 02 12:19:23 2020

Tue Jun 02 12:33:42 2020

1) 6

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	REACTIVE CN	P	-0.5974	µg/l	6/2/2020 10:35:15
5.0PPBCN	A	REACTIVE CN	P	4.5285	µg/l	6/2/2020 10:35:16
10PPBCN	A	REACTIVE CN	P	9.6871	µg/l	6/2/2020 10:35:17
50PPBCN	A	REACTIVE CN	P	50.5334	µg/l	6/2/2020 10:35:18
100PPBCN	A	REACTIVE CN	P	101.8724	µg/l	6/2/2020 10:35:19
250PPBCN	A	REACTIVE CN	P	248.7857	µg/l	6/2/2020 10:35:20
500PPBCN	A	REACTIVE CN	P	500.1903	µg/l	6/2/2020 10:35:21
ICV1	S	REACTIVE CN	P	96.8327	µg/l	6/2/2020 12:19:24
ICB1	S	REACTIVE CN	P	0.0111	µg/l	6/2/2020 12:19:25
CCV1	S	REACTIVE CN	P	242.1197	µg/l	6/2/2020 12:19:27
CCB1	S	REACTIVE CN	P	-0.0443	µg/l	6/2/2020 12:19:30
PB129215BL	S	REACTIVE CN	P	-0.164	µg/l	6/2/2020 12:19:32
L2805-02	S	REACTIVE CN	P	-0.1539	µg/l	6/2/2020 12:19:33
L2805-02DUP	S	REACTIVE CN	P	-0.1035	µg/l	6/2/2020 12:26:55
L2813-06	S	REACTIVE CN	P	0.0521	µg/l	6/2/2020 12:26:57
L2814-06	S	REACTIVE CN	P	0.1146	µg/l	6/2/2020 12:26:58
L2822-04	S	REACTIVE CN	P	0.0389	µg/l	6/2/2020 12:26:59
L2822-05	S	REACTIVE CN	P	0.1859	µg/l	6/2/2020 12:27:00
L2822-06	S	REACTIVE CN	P	0.0828	µg/l	6/2/2020 12:27:01
PB129240BL	S	REACTIVE CN	P	0.138	µg/l	6/2/2020 12:27:02
L2831-01	S	REACTIVE CN	P	0.1019	µg/l	6/2/2020 12:27:04
CCV2	S	REACTIVE CN	P	238.5905	µg/l	6/2/2020 12:33:34
CCB2	S	REACTIVE CN	P	0.1395	µg/l	6/2/2020 12:33:35
L2831-01DUP	S	REACTIVE CN	P	0.1447	µg/l	6/2/2020 12:33:37
CCV3	S	REACTIVE CN	P	243.8259	µg/l	6/2/2020 12:33:40
CCB3	S	REACTIVE CN	P	0.3751	µg/l	6/2/2020 12:33:41

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dh

Instrument ID : Konelab

6/2/2020 10:37


Test Pestic
Total CN

Accepted 6/2/2020 10:37

Factor 1206
Bias 0.003

Coeff. of det. 0.999971

Errors

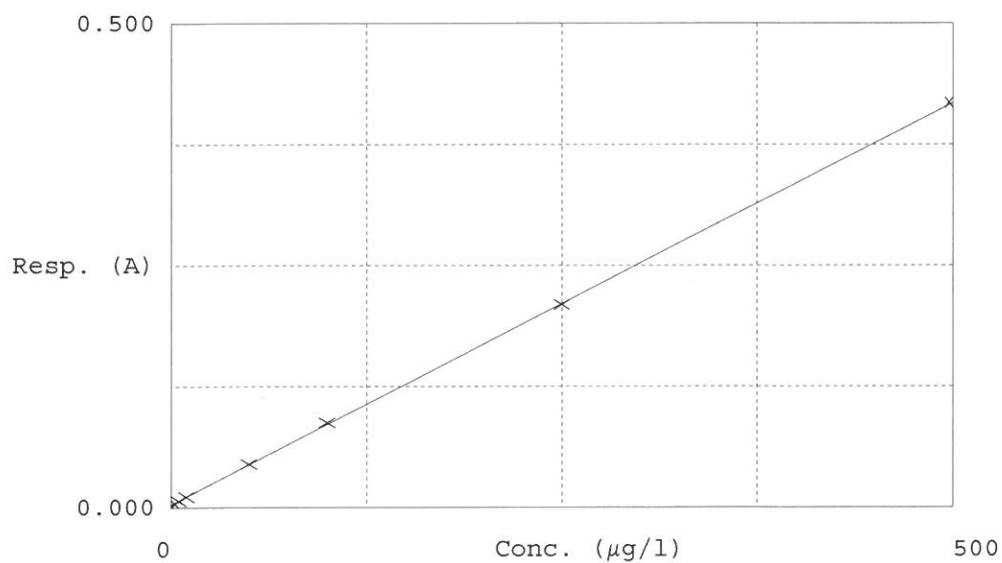

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.5974	0.0000	
2	5.0PPBCN	0.007	4.5285	5.0000	
3	10PPBCN	0.011	9.6871	10.0000	
4	50PPBCN	0.045	50.5334	50.0000	
5	100PPBCN	0.088	101.8724	100.0000	
6	250PPBCN	0.210	248.7857	250.0000	
7	500PPBCN	0.418	500.1903	500.0000	