


LB109542

7471B

INSTRUMENT ID: CV1

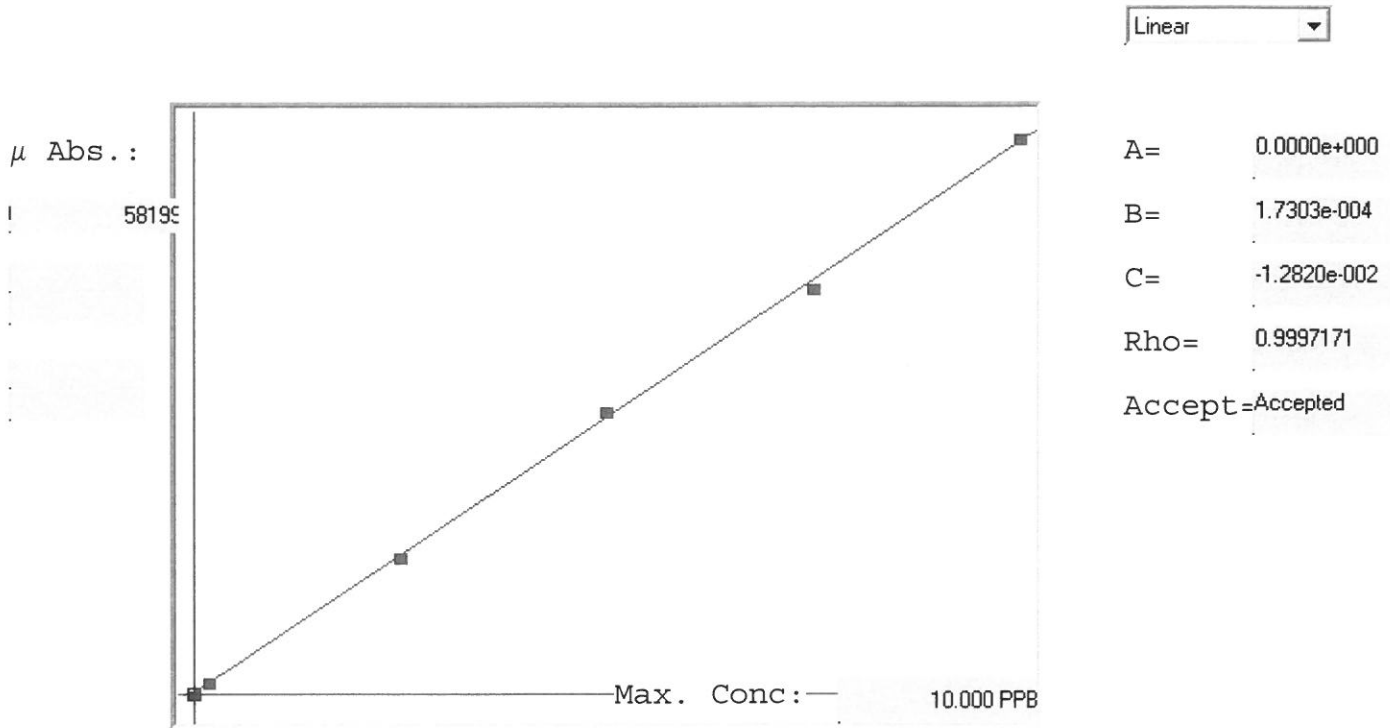

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.004	-0.004	51	0.000	51				
0.2	0.200	0.208	0.008	1279	0.0 %	1279				
2.5	2.500	2.467	-0.033	14332	0.0 %	14332				
5.0	5.000	5.129	0.129	29716	0.0 %	29716				
7.5	7.500	7.342	-0.158	42503	0.0 %	42503				
10.0	10.000	10.058	0.058	58199	0.0 %	58199				

LB109542 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 10 Jun 2020 12:59:26					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	51	-	0.0000	7471B	PPB	10 Jun 2020 13:40:45	S	Std
0.2 - 1	50.2	1279	-	0.2000	7471B	PPB	10 Jun 2020 13:43:02	S	Std
2.5 - 1	52.5	14332	-	2.5000	7471B	PPB	10 Jun 2020 13:45:19	S	Std
5.0 - 1	55	29716	-	5.0000	7471B	PPB	10 Jun 2020 13:47:37	S	Std
7.5 - 1	57.5	42503	-	7.5000	7471B	PPB	10 Jun 2020 13:49:53	S	Std
10.0 - 1	810	58199	-	10.0000	7471B	PPB	10 Jun 2020 13:52:11	S	Std
ICV78 - 1	ICV78	22911	3.9516	-	7471B	PPB	10 Jun 2020 13:55:11	U	SMPL
ICB78 - 1	ICB78	-69	-0.0248	-	7471B	PPB	10 Jun 2020 13:57:26	U	SMPL
CCV92 - 1	CCV92	29571	5.1040	-	7471B	PPB	10 Jun 2020 13:59:42	U	SMPL
CCB92 - 1	CCB92	-85	-0.0275	-	7471B	PPB	10 Jun 2020 14:01:57	U	SMPL
CRA - 1	CRA	1283	0.2092	-	7471B	PPB	10 Jun 2020 14:04:13	U	SMPL
HighStd - 1	HighStd	58180	10.0543	-	7471B	PPB	10 Jun 2020 14:06:28	U	SMPL
ChkStd - 1	ChkStd	41901	7.2375	-	7471B	PPB	10 Jun 2020 14:08:44	U	SMPL
PB129460BL - 1	PBS	-228	-0.0523	-	7471B	PPB	10 Jun 2020 14:11:01	U	SMPL
PB129460BS - 1	LCSS	20786	3.5839	-	7471B	PPB	10 Jun 2020 14:13:18	U	SMPL
L2810-01 - 1	CL-02-060920	2994	0.5052	-	7471B	PPB	10 Jun 2020 14:15:35	U	SMPL
L2810-01DUP - 1	CL-02-060920DUP	2991	0.5047	-	7471B	PPB	10 Jun 2020 14:17:52	U	SMPL
L2810-01MS - 1	CL-02-060920MS	24654	4.2532	-	7471B	PPB	10 Jun 2020 14:20:10	U	SMPL
L2810-01MSD - 1	CL-02-060920MSD	23657	4.0807	-	7471B	PPB	10 Jun 2020 14:22:27	U	SMPL
L2954-02 - 1	239-355	15944	2.7460	-	7471B	PPB	10 Jun 2020 14:24:43	U	SMPL
CCV93 - 1	CCV93	29856	5.1533	-	7471B	PPB	10 Jun 2020 14:26:59	U	SMPL
CCB93 - 1	CCB93	-78	-0.0263	-	7471B	PPB	10 Jun 2020 14:29:15	U	SMPL
L2961-01 - 1	FM-CON-1	1371	0.2244	-	7471B	PPB	10 Jun 2020 14:31:31	U	SMPL
L2961-02 - 1	FM-CON-2	8044	1.3791	-	7471B	PPB	10 Jun 2020 14:33:47	U	SMPL
L2961-03 - 1	FM-CON-3	2827	0.4763	-	7471B	PPB	10 Jun 2020 14:36:03	U	SMPL
L2961-04 - 1	FM-CON-4	2079	0.3469	-	7471B	PPB	10 Jun 2020 14:38:20	U	SMPL
L2961-05 - 1	FM-CON-5	1275	0.2078	-	7471B	PPB	10 Jun 2020 14:40:36	U	SMPL
L2810-01LX5 - 1		490	0.0720	-	7471B	PPB	10 Jun 2020 14:42:53	U	SMPL
L2810-01A - 1		27473	4.7410	-	7471B	PPB	10 Jun 2020 14:45:10	U	SMPL
CCV94 - 1	CCV94	29979	5.1746	-	7471B	PPB	10 Jun 2020 14:47:27	U	SMPL
CCB94 - 1	CCB94	-63	-0.0237	-	7471B	PPB	10 Jun 2020 14:49:45	U	SMPL