

LB109613

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dr

Instrument ID : Konelab

6/16/2020 13:46

Test: ^{penicillin} ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.919	0.0	0.081	
ICB1	-0.479	0.0	0.003	
CCV1	246.687	0.0	0.199	
CCB1	-0.216	0.0	0.003	
PB129548BL	-0.170	0.0	0.004	
L2808-05	0.287	0.0	0.004	
L2808-05DUP	-0.948	0.0	0.003	
L2997-02	-0.712	0.0	0.003	
L2998-01	-0.624	0.0	0.003	
L3013-02	-0.578	0.0	0.003	
L3013-04	-0.443	0.0	0.003	
CCV2	249.518	0.0	0.202	
CCB2	-0.648	0.0	0.003	

N	13
Mean	45.353
SD	93.9703
CV%	207.20

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 16 13:31:17 2020

Tue Jun 16 13:38:33 2020

Ja

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	-1.0955	µg/l	6/16/2020 11:15:08
5.OPPBCN	A	REACTIVE CN	P	3.8683	µg/l	6/16/2020 11:15:09
10PPBCN	A	REACTIVE CN	P	9.0823	µg/l	6/16/2020 11:15:10
50PPBCN	A	REACTIVE CN	P	50.0869	µg/l	6/16/2020 11:15:11
100PPBCN	A	REACTIVE CN	P	101.0571	µg/l	6/16/2020 11:15:12
250PPBCN	A	REACTIVE CN	P	254.3827	µg/l	6/16/2020 11:15:13
500PPBCN	A	REACTIVE CN	P	497.6182	µg/l	6/16/2020 11:15:14
ICV1	S	REACTIVE CN	P	97.9192	µg/l	6/16/2020 13:31:18
ICB1	S	REACTIVE CN	P	-0.479	µg/l	6/16/2020 13:31:19
CCV1	S	REACTIVE CN	P	246.687	µg/l	6/16/2020 13:31:21
CCB1	S	REACTIVE CN	P	-0.2161	µg/l	6/16/2020 13:31:24
PB129548BL	S	REACTIVE CN	P	-0.17	µg/l	6/16/2020 13:31:25
L2808-05	S	REACTIVE CN	P	0.287	µg/l	6/16/2020 13:31:27
L2808-05DUP	S	REACTIVE CN	P	-0.9481	µg/l	6/16/2020 13:38:24
L2997-02	S	REACTIVE CN	P	-0.7118	µg/l	6/16/2020 13:38:26
L2998-01	S	REACTIVE CN	P	-0.6237	µg/l	6/16/2020 13:38:27
L3013-02	S	REACTIVE CN	P	-0.5781	µg/l	6/16/2020 13:38:28
L3013-04	S	REACTIVE CN	P	-0.4427	µg/l	6/16/2020 13:38:29
CCV2	S	REACTIVE CN	P	249.5182	µg/l	6/16/2020 13:38:31
CCB2	S	REACTIVE CN	P	-0.6484	µg/l	6/16/2020 13:38:33

LB109613

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : OK

Instrument ID : Konelab

6/16/2020 11:59


Test ^{Prucha}
~~Total~~ CN

Accepted 6/16/2020 11:59

Factor 1260
Bias 0.004

Coeff. of det. 0.999857

Errors

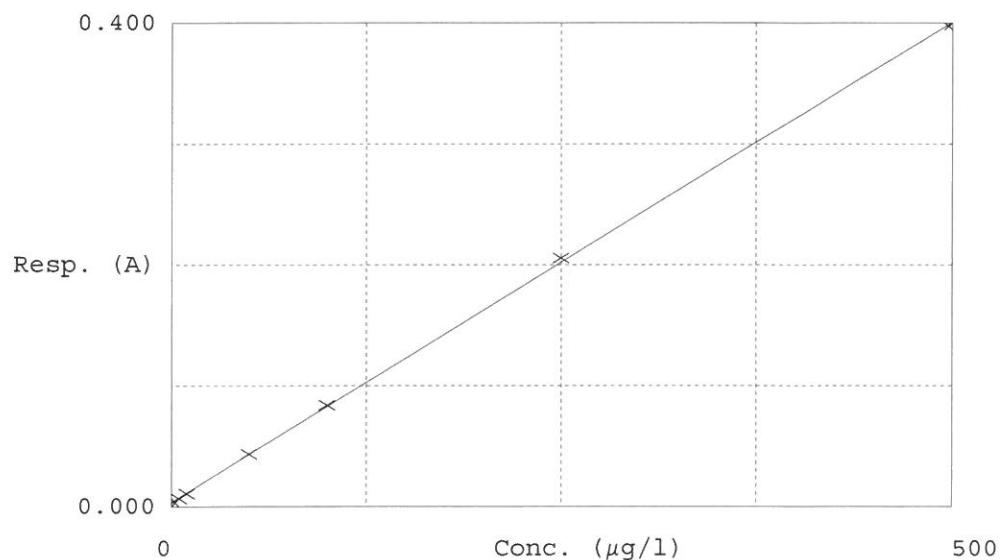

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.0955	0.0000	
2	5.0PPBCN	0.007	3.8683	5.0000	
3	10PPBCN	0.011	9.0823	10.0000	
4	50PPBCN	0.043	50.0869	50.0000	
5	100PPBCN	0.084	101.0571	100.0000	
6	250PPBCN	0.206	254.3827	250.0000	
7	500PPBCN	0.399	497.6182	500.0000	