


LB109623

7471B

INSTRUMENT ID: CY1

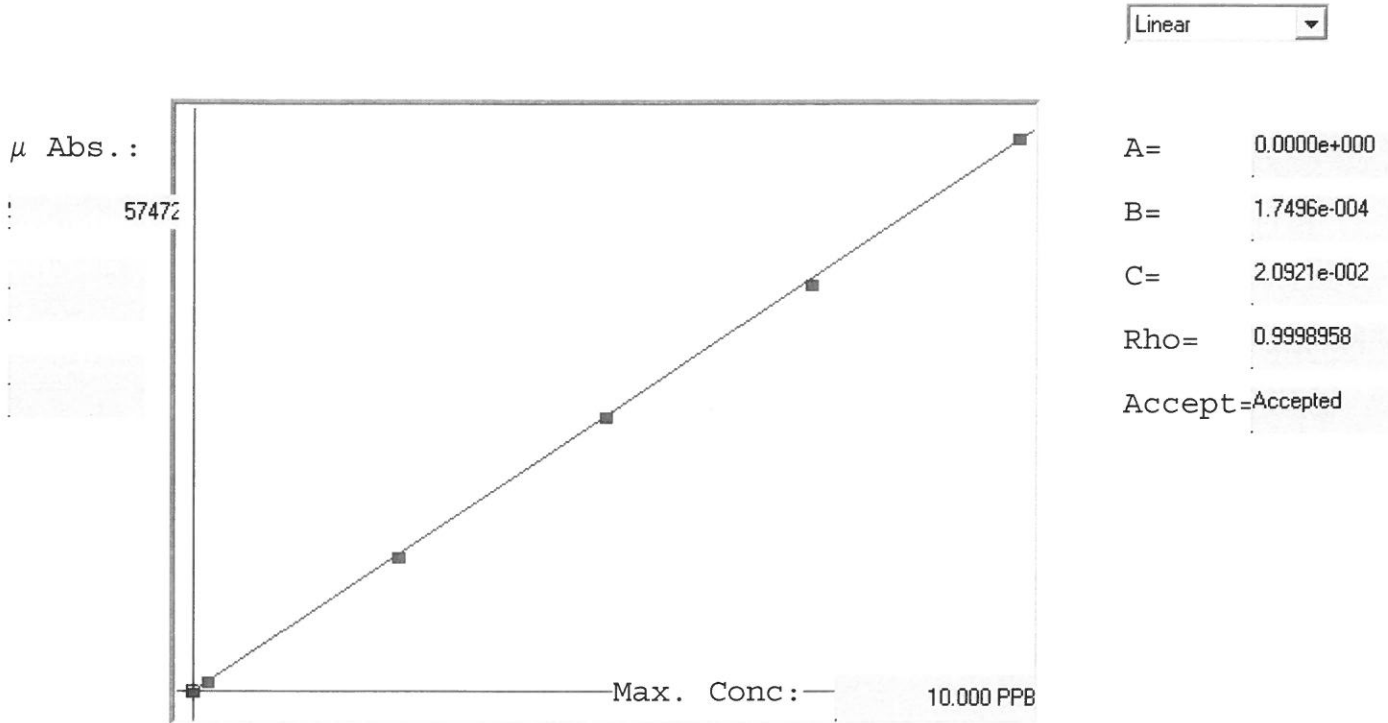

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.020	0.020	-3	0.000	-3				
0.2	0.200	0.220	0.020	1140	0.0 %	1140				
2.5	2.500	2.479	-0.021	14052	0.0 %	14052				
5.0	5.000	5.003	0.003	28478	0.0 %	28478				
7.5	7.500	7.400	-0.100	42177	0.0 %	42177				
10.0	10.000	10.076	0.076	57472	0.0 %	57472				

LB109623 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 17 Jun 2020 10:32:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-3	-	0.00007471B	PPB		17 Jun 2020 10:42:36	S	Std
0.2 - 1	50.2	1140	-	0.20007471B	PPB		17 Jun 2020 10:44:53	S	Std
2.5 - 1	52.5	14052	-	2.50007471B	PPB		17 Jun 2020 10:47:10	S	Std
5.0 - 1	55	28478	-	5.00007471B	PPB		17 Jun 2020 10:49:27	S	Std
7.5 - 1	57.5	42177	-	7.50007471B	PPB		17 Jun 2020 10:51:44	S	Std
10.0 - 1	510	57472	-	10.00007471B	PPB		17 Jun 2020 10:59:07	S	Std
ICV87 - 1	ICV87	23072	4.0576	-7471B	PPB		17 Jun 2020 11:02:00	U	SMPL
ICB87 - 1	ICB87	-91	0.0050	-7471B	PPB		17 Jun 2020 11:04:15	U	SMPL
CCV30 - 1	CCV30	28819	5.0631	-7471B	PPB		17 Jun 2020 11:06:31	U	SMPL
CCB30 - 1	CCB30	-102	0.0031	-7471B	PPB		17 Jun 2020 11:08:46	U	SMPL
CRA - 1	CRA	1128	0.2183	-7471B	PPB		17 Jun 2020 11:11:02	U	SMPL
HighStd - 1	HighStd	58253	10.2128	-7471B	PPB		17 Jun 2020 11:13:17	U	SMPL
ChkStd - 1	ChkStd	40427	7.0940	-7471B	PPB		17 Jun 2020 11:15:32	U	SMPL
PB129583BL - 1	PBS	-147	-0.0048	-7471B	PPB		17 Jun 2020 11:17:50	U	SMPL
PB129583BS - 1	LCSS	21976	3.8658	-7471B	PPB		17 Jun 2020 11:20:08	U	SMPL
L2811-01 - 1	NB-08-061220	5192	0.9293	-7471B	PPB		17 Jun 2020 11:22:24	U	SMPL
L2930-01 - 1	S39-HSVE2-IDW01	109	0.0400	-7471B	PPB		17 Jun 2020 11:27:31	U	SMPL
L2930-02 - 1	S39-HSVE3-IDW01	166	0.0500	-7471B	PPB		17 Jun 2020 11:33:25	U	SMPL
L3022-02 - 1	HLP-A	1517	0.2863	-7471B	PPB		17 Jun 2020 11:35:42	U	SMPL
L3022-02DUP - 1	HLP-ADUP	1558	0.2935	-7471B	PPB		17 Jun 2020 11:37:57	U	SMPL
CCV31 - 1	CCV31	28647	5.0330	-7471B	PPB		17 Jun 2020 11:40:12	U	SMPL
CCB31 - 1	CCB31	-80	0.0069	-7471B	PPB		17 Jun 2020 11:42:27	U	SMPL
L3022-02MS - 1	HLP-AMS	22894	4.0264	-7471B	PPB		17 Jun 2020 11:44:42	U	SMPL
L3022-02MSD - 1	HLP-AMSD	22919	4.0308	-7471B	PPB		17 Jun 2020 11:46:58	U	SMPL
L3022-04 - 1	HLP-B	1177	0.2268	-7471B	PPB		17 Jun 2020 11:49:14	U	SMPL
L3023-01 - 1	339	439	0.0977	-7471B	PPB		17 Jun 2020 11:51:30	U	SMPL
L3030-01 - 1	SB-01(8-10)	172	0.0510	-7471B	PPB		17 Jun 2020 11:53:46	U	SMPL
L3022-02LX5 - 1		274	0.0689	-7471B	PPB		17 Jun 2020 11:56:03	U	SMPL
L3022-02A - 1		26310	4.6241	-7471B	PPB		17 Jun 2020 11:58:19	U	SMPL
CCV32 - 1	CCV32	27729	4.8724	-7471B	PPB		17 Jun 2020 12:00:36	U	SMPL
CCB32 - 1	CCB32	-101	0.0033	-7471B	PPB		17 Jun 2020 12:02:54	U	SMPL